

Quality Assessment Scheme for Acetylcholine receptor autoantibodies

The results from all participants can be found in the outstanding table, listed according to their Lab Number.

| Method | all | commercial kits | | | | In house assay none (nmol/L) |
|----------------|------|-----------------|----------|-----------|----------|------------------------------|
| | | IBL | RSR RIA | RSR ELISA | other | |
| Cut-off | | >0.4 | ≥0.5 | ≥0.45 | ≥0.5 | |
| Number of lab. | | (nmol/L) | (nmol/L) | (nmol/L) | (nmol/L) | |
| 131 | 0,32 | 0,32 | | | | |
| 194 | 0,39 | 0,39 | | | | |
| 199 | 0,39 | 0,39 | | | | |
| 207 | 2,49 | | | | 2,49 | |
| 242 | 0,79 | | 0,79 | | | |
| 379 | 0,38 | 0,38 | | | | |
| 381 | 0,39 | 0,39 | | | | |
| 382 | 0,70 | | | | | 0,70 |
| 384 | 1,10 | 1,10 | | | | |
| 385 | 1,70 | | 1,70 | | | |
| 389 | 0,40 | 0,40 | | | | |
| 393 | 0,42 | 0,42 | | | | |
| 397 | 0,32 | 0,32 | | | | |
| 398 | 0,35 | 0,35 | | | | |
| 399 | 0,41 | 0,41 | | | | |
| 401 | 1,74 | | | 1,74 | | |
| 402 | 0,32 | 0,32 | | | | |
| 403 | 0,45 | 0,45 | | | | |
| 406 | 0,33 | 0,33 | | | | |
| 412 | 0,35 | 0,35 | | | | |
| 414 | 0,38 | 0,38 | | | | |
| 418 | 0,50 | | 0,50 | | | |
| 421 | 0,72 | | | | 0,72 | |
| 423 | 0,90 | | | | 0,90 | |
| 425 | 0,35 | 0,35 | | | | |
| 426 | 0,38 | 0,38 | | | | |
| 428 | 1,90 | | | 1,90 | | |

Statistical Results Sample Number 25-1A:

| Method | all | commercial kits | | | | In house assay |
|------------|------|-----------------|---------|-----------|-------|----------------|
| | | IBL | RSR RIA | RSR ELISA | other | |
| Mean | 0,70 | 0,41 | 1,00 | 1,82 | 1,37 | 0,70 |
| SD | 0,58 | 0,18 | 0,63 | 0,11 | 0,97 | - |
| Mean - 2SD | <0 | 0,06 | <0 | 1,59 | <0 | - |
| Mean + 2SD | 1,86 | 0,76 | 2,25 | 2,05 | 3,32 | - |
| Amount | 27 | 18 | 3 | 2 | 3 | 1 |


Samples have been determined by the single collectives as described below:

IBL

Negative < 0.25 nmol/L

Positive > 0.40 nmol/L


Equivocal 0.25 – 0.40 nmol/L

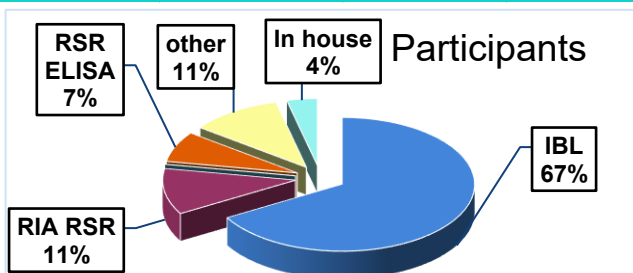

*The graphic is for information purposes only and not validated. Please read your results from the table.

Statistical Results Sample Number 25-1A:

| Method | all | commercial kits | | | | In house assay |
|-----------|-----|-----------------|---------|-----------|-------|----------------|
| | | IBL | RSR RIA | RSR ELISA | other | |
| Negative | 1 | 1 | - | - | - | - |
| Equivocal | 14 | 12 | 1 | 1 | - | - |
| Positive | 12 | 5 | 2 | 1 | 3 | 1 |
| Amount | 27 | 18 | 3 | 2 | 3 | 1 |

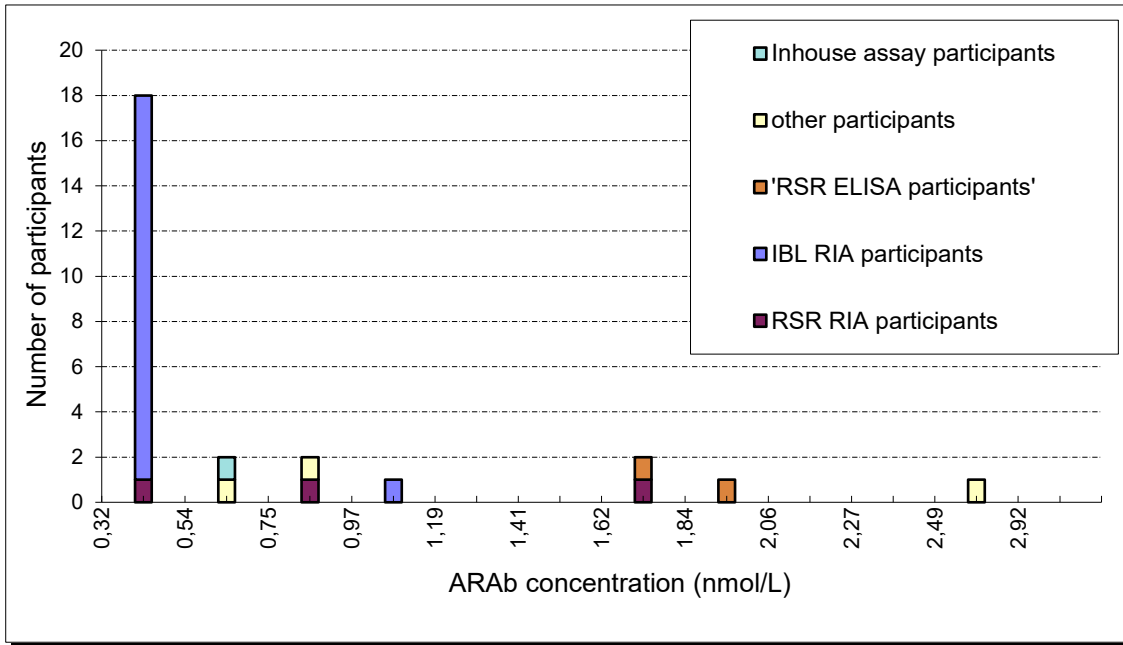

***The graphic is for information purposes only and not validated. Please read your results from the table.**

The results from all participants can be found in the outstanding table, listed according to their Lab Number.


Statistical Results Sample Number 25-1B:

| Method | all | commercial kits | | | | In house assay none (nmol/L) |
|----------------|------|-----------------|------------------|--------------------|----------------|------------------------------|
| | | IBL (nmol/L) | RSR RIA (nmol/L) | RSR ELISA (nmol/L) | other (nmol/L) | |
| Cut-off | | >0.4 | >0.5 | >0.45 | >0.5 | |
| Number of lab. | | (nmol/L) | (nmol/L) | (nmol/L) | (nmol/L) | (nmol/L) |
| 131 | 0,25 | 0,25 | | | | |
| 194 | 0,20 | 0,20 | | | | |
| 199 | 0,12 | 0,12 | | | | |
| 207 | 0,16 | | | | 0,16 | |
| 242 | 0,25 | | 0,25 | | | |
| 379 | 0,07 | 0,07 | | | | |
| 381 | 0,02 | 0,02 | | | | |
| 382 | 0,00 | | | | | 0,00 |
| 384 | 0,10 | 0,10 | | | | |
| 385 | 0,30 | | 0,30 | | | |
| 389 | 0,00 | 0,00 | | | | |
| 393 | 0,03 | 0,03 | | | | |
| 397 | 0,20 | 0,20 | | | | |
| 398 | 0,25 | 0,25 | | | | |
| 399 | 0,10 | 0,10 | | | | |
| 401 | 0,45 | | | 0,45 | | |
| 402 | 0,07 | 0,07 | | | | |
| 403 | 0,20 | 0,20 | | | | |
| 406 | 0,25 | 0,25 | | | | |
| 412 | 0,25 | 0,25 | | | | |
| 414 | 0,20 | 0,20 | | | | |
| 418 | 0,10 | | 0,10 | | | |
| 421 | 0,10 | | | | 0,10 | |
| 423 | 0,00 | | | | 0,00 | |
| 425 | 0,25 | 0,25 | | | | |
| 426 | 0,20 | 0,20 | | | | |
| 428 | 0,39 | | | 0,39 | | |

| Method | all | commercial kits | | | | In house assay |
|------------|------|-----------------|---------|-----------|-------|----------------|
| | | IBL | RSR RIA | RSR ELISA | other | |
| Mean | 0,17 | 0,15 | 0,22 | 0,42 | 0,09 | 0,00 |
| SD | 0,12 | 0,09 | 0,10 | 0,04 | 0,08 | - |
| Mean - 2SD | <0 | <0 | 0,01 | 0,34 | <0 | - |
| Mean + 2SD | 0,40 | 0,33 | 0,42 | 0,50 | 0,25 | - |
| Amount | 27 | 17 | 3 | 2 | 3 | 1 |

Samples have been determined by the single collectives as described below:


Negative < 0.25 nmol/L
 Positive > 0.40 nmol/L
 Equivocal 0.25 – 0.40 nmol/L



***The graphic is for information purposes only and not validated. Please read your results from the table.**

Statistical Results Sample Number 25-1B:

| Method | all | commercial kits | | | | In house assay |
|-----------|-----|-----------------|---------|-----------|-------|----------------|
| | | IBL | RSR RIA | RSR ELISA | other | |
| Negative | 27 | 18 | 3 | 2 | 3 | 1 |
| Equivocal | 0 | - | - | - | - | - |
| Positive | 0 | - | - | - | - | - |
| Amount | 27 | 18 | 3 | 2 | 3 | 1 |

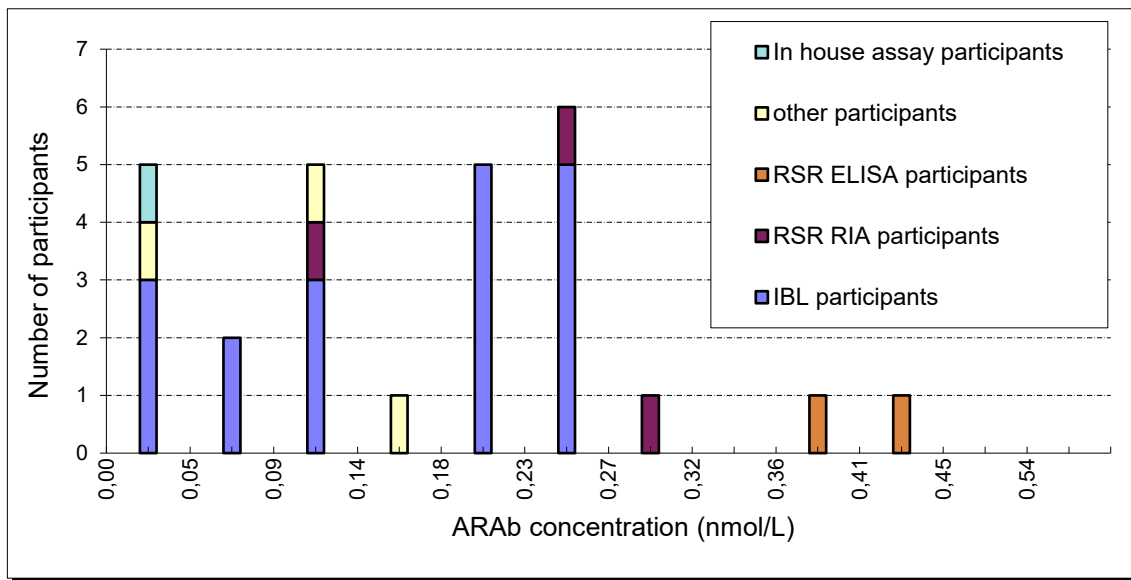

***The graphic is for information purposes only and not validated. Please read your results from the table.**

The results from all participants can be found in the outstanding table, listed according to their Lab Number.

Statistical Results Sample Number 25-1C:


| Method | all | commercial kits | | | | In house assay |
|----------------|------|-----------------|----------|-----------|----------|----------------|
| | | IBL | RSR RIA | RSR ELISA | other | |
| Cut-off | | >0.4 | ≥0.5 | ≥0.45 | ≥0.5 | none |
| Number of lab. | | (nmol/L) | (nmol/L) | (nmol/L) | (nmol/L) | (nmol/L) |
| 131 | 1,20 | 1,20 | | | | |
| 194 | 1,30 | 1,30 | | | | |
| 199 | 1,08 | 1,08 | | | | |
| 207 | 8,28 | | | | 8,28 | |
| 242 | 2,34 | | 2,34 | | | |
| 379 | 1,20 | 1,20 | | | | |
| 381 | 1,18 | 1,18 | | | | |
| 382 | 2,10 | | | | | 2,10 |
| 384 | 3,20 | 3,20 | | | | |
| 385 | 4,00 | | 4,00 | | | |
| 389 | 1,58 | 1,58 | | | | |
| 393 | 1,18 | 1,18 | | | | |
| 397 | 1,01 | 1,01 | | | | |
| 398 | 1,20 | 1,20 | | | | |
| 399 | 1,14 | 1,14 | | | | |
| 401 | 6,09 | | | 6,09 | | |
| 402 | 1,06 | 1,06 | | | | |
| 403 | 1,20 | 1,20 | | | | |
| 406 | 1,20 | 1,20 | | | | |
| 412 | 1,10 | 1,10 | | | | |
| 414 | 1,25 | 1,25 | | | | |
| 418 | 2,40 | | 2,40 | | | |
| 421 | 2,35 | | | | 2,35 | |
| 423 | 2,40 | | | | 2,40 | |
| 425 | 1,10 | 1,10 | | | | |
| 426 | 1,16 | 1,16 | | | | |
| 428 | 7,50 | | | 7,50 | | |

Statistical Results Sample Number 25-1C:

| Method | all | commercial kits | | | | In house assay |
|------------|------|-----------------|---------|-----------|-------|----------------|
| | | IBL | RSR RIA | RSR ELISA | other | |
| Mean | 2,25 | 1,30 | 2,91 | 6,80 | 4,34 | 2,10 |
| SD | 1,98 | 0,49 | 0,94 | 1,00 | 3,41 | - |
| Mean - 2SD | <0 | 0,32 | 1,03 | 4,80 | <0 | - |
| Mean + 2SD | 6,22 | 2,28 | 4,80 | 8,79 | 11,16 | - |
| Amount | 27 | 17 | 3 | 2 | 3 | 1 |

Samples have been determined by the single collectives as described below:


Negative < 0.25 nmol/L
 Positive > 0.40 nmol/L
 Equivocal 0.25 – 0.40 nmol/L



*The graphic is for information purposes only and not validated. Please read your results from the table.

Statistical Results Sample Number 25-1C:

| Method | all | commercial kits | | | | In house assay |
|-----------|-----|-----------------|---------|-----------|-------|----------------|
| | | IBL | RSR RIA | RSR ELISA | other | |
| Negative | 0 | - | - | - | - | - |
| Equivocal | 0 | - | - | - | - | - |
| Positive | 27 | 18 | 3 | 2 | 3 | 1 |
| Amount | 27 | 18 | 3 | 2 | 3 | 1 |



*The graphic is for information purposes only and not validated. Please read your results from the table.