




Statistical Results Sample Number 21-2A:


Method	all	commercial kits					In house
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	assay
Mean	0,15	0,11	0,20	-	0,62	0,13	0,00
SD	0,17	0,10	-	-	-	0,15	-
Mean - 2SD	<0	<0	-	-	-	<0	-
Mean + 2SD	0,49	0,30	-	-	-	0,44	-
Amount	26	19	1	0	2	3	1

Samples have been determined by the single collectives as described below:  
 IBL  
 Negative < 0.25 nmol/L  
 Positive > 0.40 nmol/L  
 Equivocal 0.25 – 0.40 nmol/L

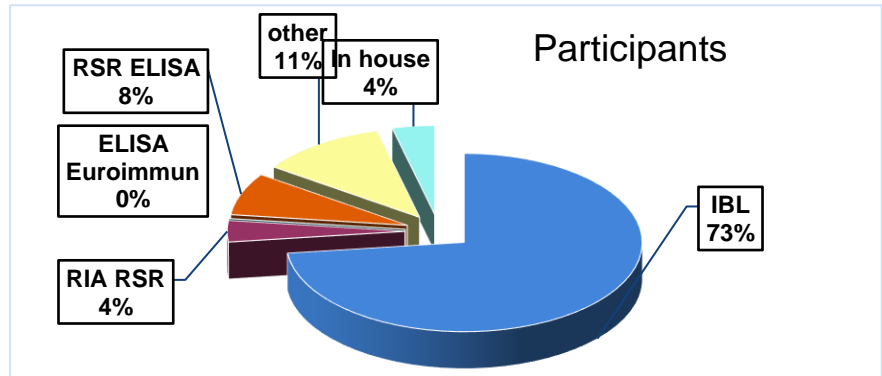

\*The graphic is for information purposes only and not validated. Please read your results from the table.

Method	all	commercial kits					In house
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	assay
Negative	24	19	1	0	1	2	1
Equivocal	2	0	0	0	1	1	0
Positive	0	0	0	0	0	0	0
Amount	26	19	1	0	2	3	1

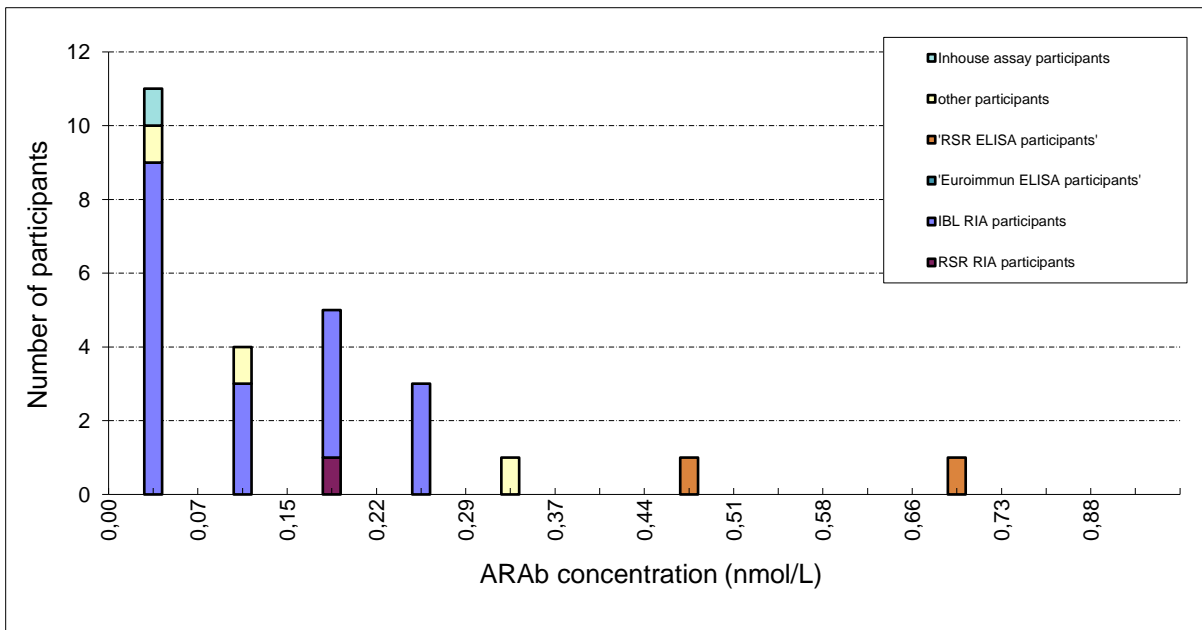

\*The graphic is for information purposes only and not validated. Please read your results from the table.




Statistical Results Sample Number 21-2B:

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Mean	0,71	0,39	-	-	3,42	1,01	0,50
SD	0,85	0,06	-	-	-	0,38	-
Mean - 2SD	<0	0,27	-	-	-	0,26	-
Mean + 2SD	2,41	0,52	-	-	-	1,77	-
Amount	25	19	0	0	2	3	1


Samples have been determined by the single collectives as described below:

Negative < 0.25 nmol/L  
 Positive > 0.40 nmol/L  
 Equivocal 0.25 – 0.40 nmol/L

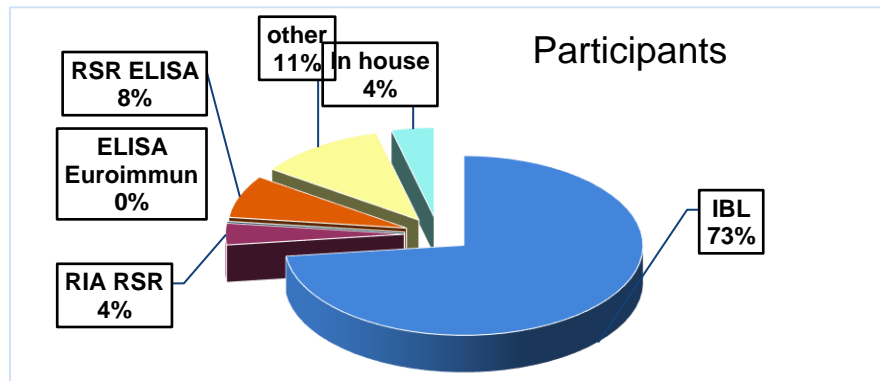

\*The graphic is for information purposes only and not validated. Please read your results from the table.

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Negative	1	1	0	0	0	0	0
Equivocal	14	13	0	0	1	0	0
Positive	10	5	0	0	1	3	1
Amount	25	19	0	0	2	3	1

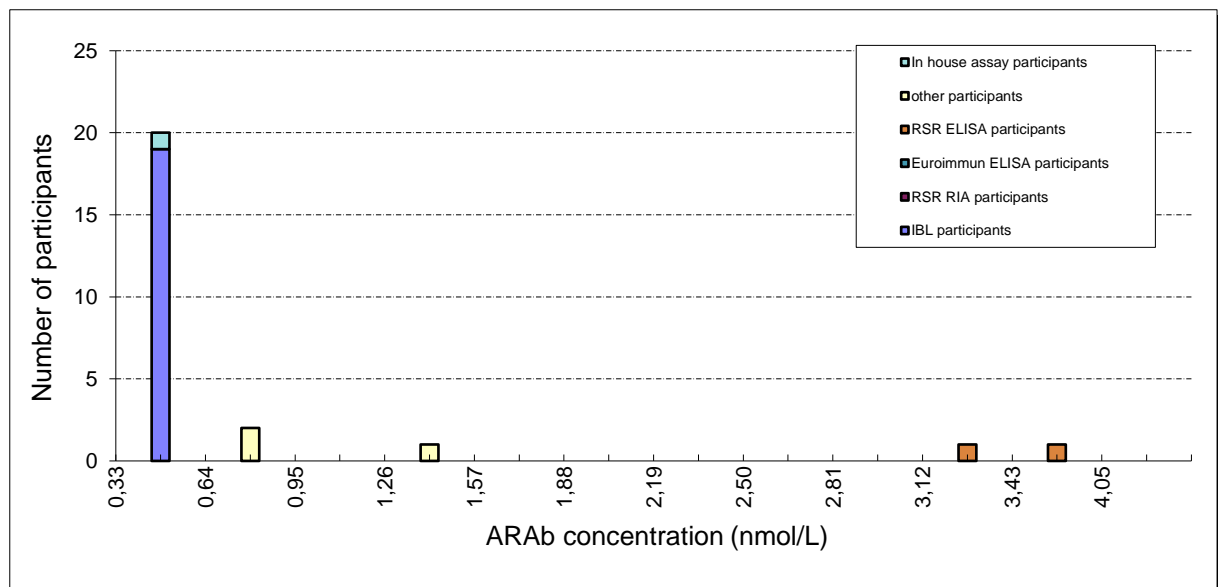

\*The graphic is for information purposes only and not validated. Please read your results from the table.




Statistical Results Sample Number 21-2C:

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Mean	1,11	0,61	1,80	-	5,11	1,46	1,00
SD	1,28	0,20	-	-	-	0,47	-
Mean - 2SD	<0	0,21	-	-	-	0,53	-
Mean + 2SD	3,67	1,00	-	-	-	2,39	-
Amount	26	19	1	0	2	3	1


Samples have been determined by the single collectives as described below:

Negative < 0.25 nmol/L  
 Positive > 0.40 nmol/L  
 Equivocal 0.25 – 0.40 nmol/L

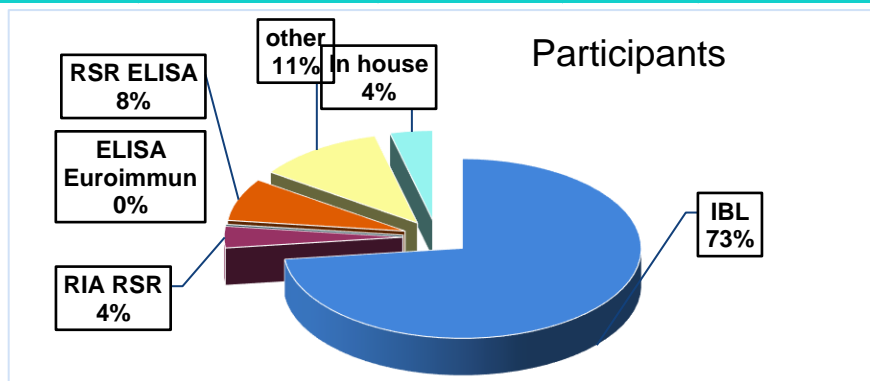

\*The graphic is for information purposes only and not validated. Please read your results from the table.

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Negative	0	0	0	0	0	0	0
Equivocal	0	0	0	0	0	0	0
Positive	26	19	1	0	2	3	1
Amount	26	19	1	0	2	3	1

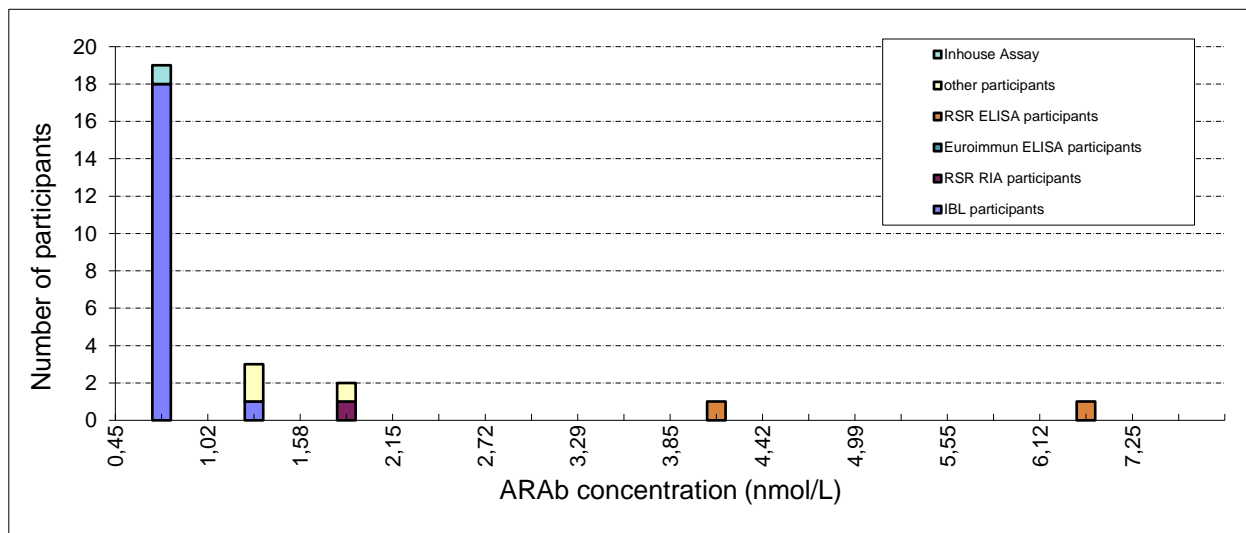

\*The graphic is for information purposes only and not validated. Please read your results from the table.