




Statistical Results Sample Number 22-1A:

Method	all	commercial kits					In house
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	assay
Mean	<b>0,69</b>	<b>0,41</b>	<b>0,87</b>	-	<b>2,95</b>	<b>0,82</b>	<b>0,40</b>
SD	<b>0,75</b>	<b>0,11</b>	<b>0,15</b>	-	-	-	-
Mean - 2SD	<b>&lt;0</b>	<b>0,18</b>	<b>0,56</b>	-	-	-	-
Mean + 2SD	<b>2,18</b>	<b>0,64</b>	<b>1,17</b>	-	-	-	-
Amount	<b>26</b>	<b>18</b>	<b>3</b>	<b>0</b>	<b>2</b>	<b>2</b>	<b>1</b>


Samples have been determined by the single collectives as described below:

IBL	
Negative	< 0.25 nmol/L
Positive	> 0.40 nmol/L
Equivocal	0.25 – 0.40 nmol/L



\*The graphic is for information purposes only and not validated. Please read your results from the table.

Method	all	commercial kits					In house
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	assay
Negative	<b>2</b>	<b>1</b>	<b>0</b>	<b>0</b>	<b>0</b>	<b>0</b>	<b>1</b>
Equivocal	<b>14</b>	<b>12</b>	<b>1</b>	<b>0</b>	<b>1</b>	<b>0</b>	<b>0</b>
Positive	<b>10</b>	<b>5</b>	<b>2</b>	<b>0</b>	<b>1</b>	<b>2</b>	<b>0</b>
Amount	<b>26</b>	<b>18</b>	<b>3</b>	<b>0</b>	<b>2</b>	<b>2</b>	<b>1</b>



\*The graphic is for information purposes only and not validated. Please read your results from the table.




Statistical Results Sample Number 22-1B:

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Mean	0,13	0,12	0,12	-	0,31	0,10	0,00
SD	0,10	0,09	0,04	-	-	-	-
Mean - 2SD	<0	<0	0,04	-	-	-	-
Mean + 2SD	0,34	0,31	0,20	-	-	-	-
Amount	26	18	3	0	2	2	1


Samples have been determined by the single collectives as described below:

Negative < 0.25 nmol/L  
 Positive > 0.40 nmol/L  
 Equivocal 0.25 – 0.40 nmol/L



\*The graphic is for information purposes only and not validated. Please read your results from the table.

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Negative	26	18	3	0	2	2	1
Equivocal	0	0	0	0	0	0	0
Positive	0	0	0	0	0	0	0
Amount	26	18	3	0	2	2	1



\*The graphic is for information purposes only and not validated. Please read your results from the table.




Statistical Results Sample Number 22-1C:

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Mean	3,11	2,09	5,02	-	7,89	4,59	3,10
SD	1,98	0,83	1,61	-	-	-	-
Mean - 2SD	<0	0,44	1,81	-	-	-	-
Mean + 2SD	7,07	3,74	8,23	-	-	-	-
Amount	26	18	3	0	2	2	1


Samples have been determined by the single collectives as described below:

Negative < 0.25 nmol/L  
 Positive > 0.40 nmol/L  
 Equivocal 0.25 – 0.40 nmol/L



\*The graphic is for information purposes only and not validated. Please read your results from the table.

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Negative	0	0	0	0	0	0	0
Equivocal	0	0	0	0	0	0	0
Positive	26	18	3	0	2	2	1
Amount	26	18	3	0	2	2	1

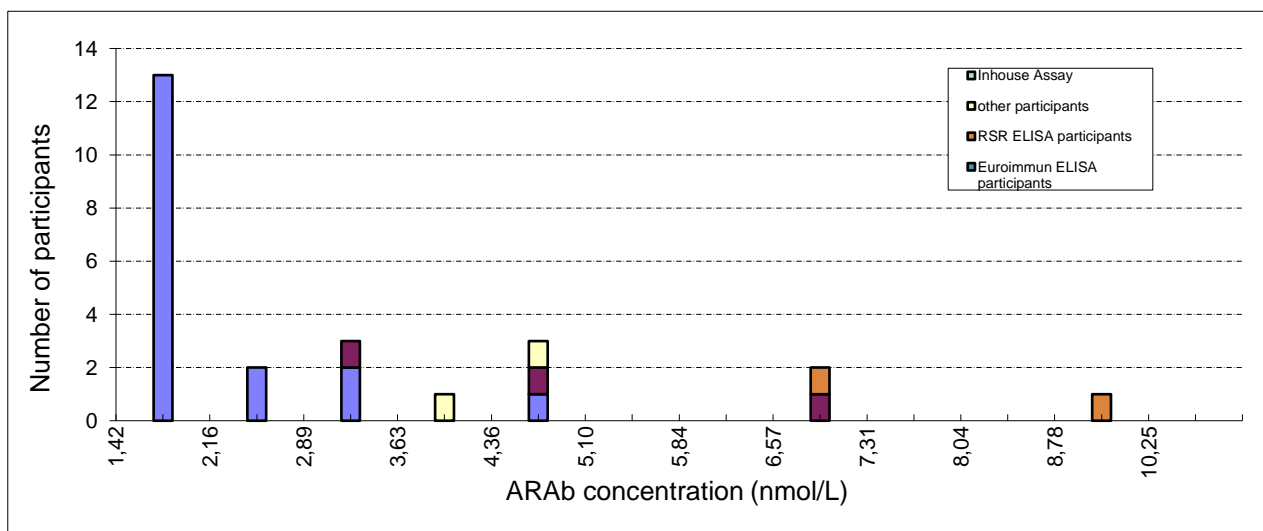

\*The graphic is for information purposes only and not validated. Please read your results from the table.