


Statistical Results Sample Number 22-2A:


Method	all	commercial kits					In house
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	assay
Mean	0,10	0,10	0,10	-	0,12	0,10	0,00
SD	0,09	0,09	0,07	-	-	-	-
Mean - 2SD	<0	<0	<0	-	-	-	-
Mean + 2SD	0,28	0,29	0,24	-	-	-	-
Amount	26	17	5	0	2	1	1

Samples have been determined by the single collectives as described below:
 IBL
 Negative < 0.25 nmol/L
 Positive > 0.40 nmol/L
 Equivocal 0.25 – 0.40 nmol/L

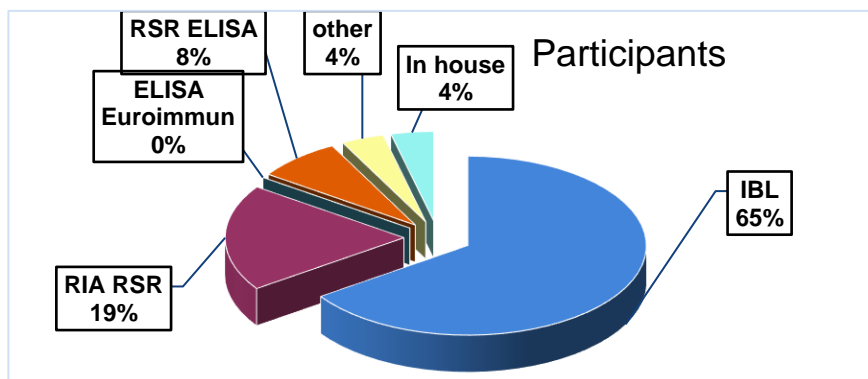

*The graphic is for information purposes only and not validated. Please read your results from the table.

Method	all	commercial kits					In house
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	assay
Negative	26	17	5	0	2	1	1
Equivocal	0	0	0	0	0	0	0
Positive	0	0	0	0	0	0	0
Amount	26	17	5	0	2	1	1

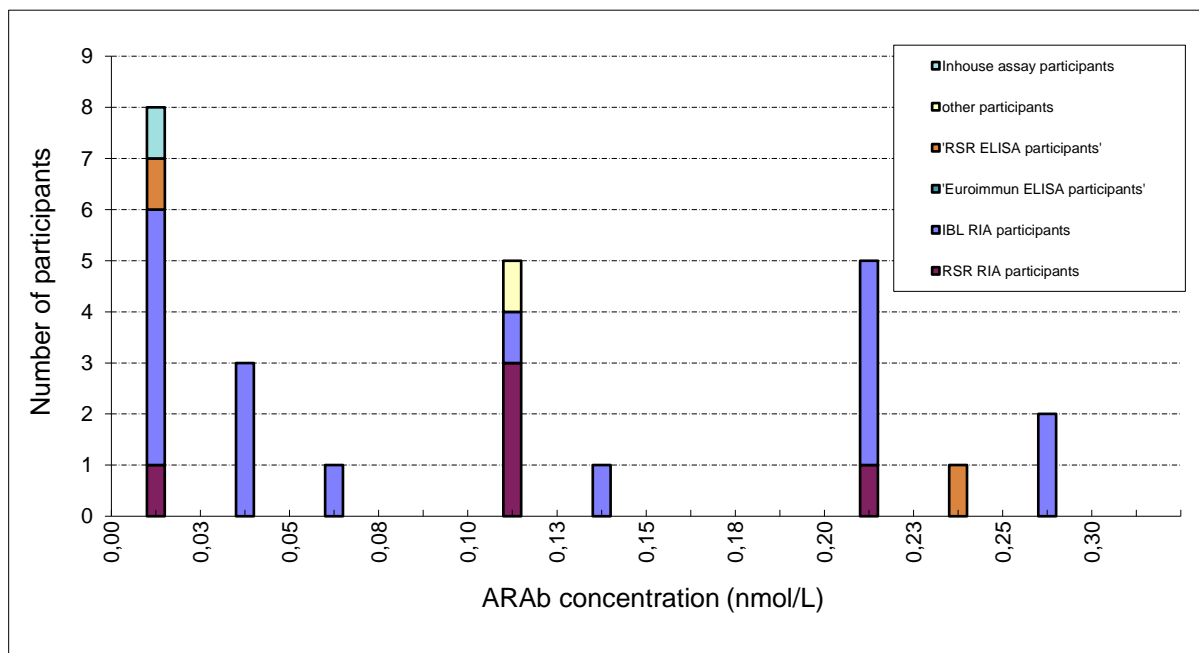


*The graphic is for information purposes only and not validated. Please read your results from the table.

Statistical Results Sample Number 22-2B:

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Mean	2,03	1,20	3,37	-	5,28	3,09	2,00
SD	1,34	0,11	0,64	-	-	-	-
Mean - 2SD	<0	0,97	2,10	-	-	-	-
Mean + 2SD	4,71	1,42	4,65	-	-	-	-
Amount	26	17	5	0	2	1	1


Samples have been determined by the single collectives as described below:

Negative < 0.25 nmol/L
 Positive > 0.40 nmol/L
 Equivocal 0.25 – 0.40 nmol/L

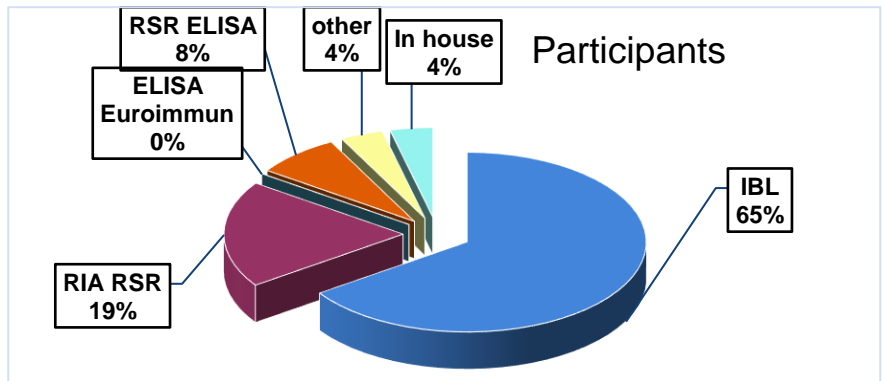

*The graphic is for information purposes only and not validated. Please read your results from the table.

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Negative	0	0	0	0	0	0	0
Equivocal	0	0	0	0	0	0	0
Positive	26	17	5	0	2	1	1
Amount	26	17	5	0	2	1	1

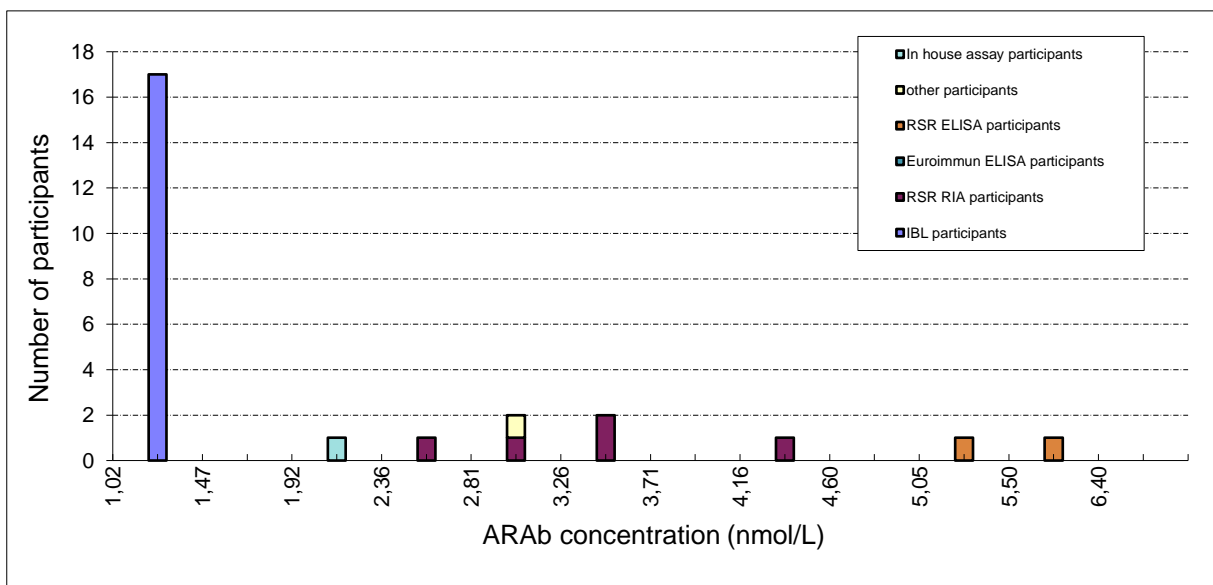


*The graphic is for information purposes only and not validated. Please read your results from the table.

Statistical Results Sample Number 22-2C:

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Mean	0,62	0,37	0,91	-	1,78	0,86	0,70
SD	0,42	0,03	0,14	-	-	-	-
Mean - 2SD	<0	0,30	0,63	-	-	-	-
Mean + 2SD	1,46	0,44	1,19	-	-	-	-
Amount	26	17	5	0	2	1	1


Samples have been determined by the single collectives as described below:

Negative < 0.25 nmol/L
 Positive > 0.40 nmol/L
 Equivocal 0.25 – 0.40 nmol/L

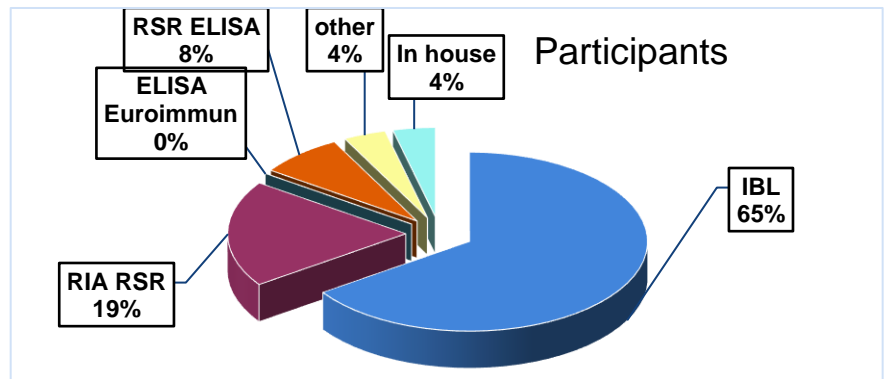

*The graphic is for information purposes only and not validated. Please read your results from the table.

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Negative	1	1	0	0	0	0	0
Equivocal	18	15	1	0	2	0	0
Positive	7	1	4	0	0	1	1
Amount	26	17	5	0	2	1	1

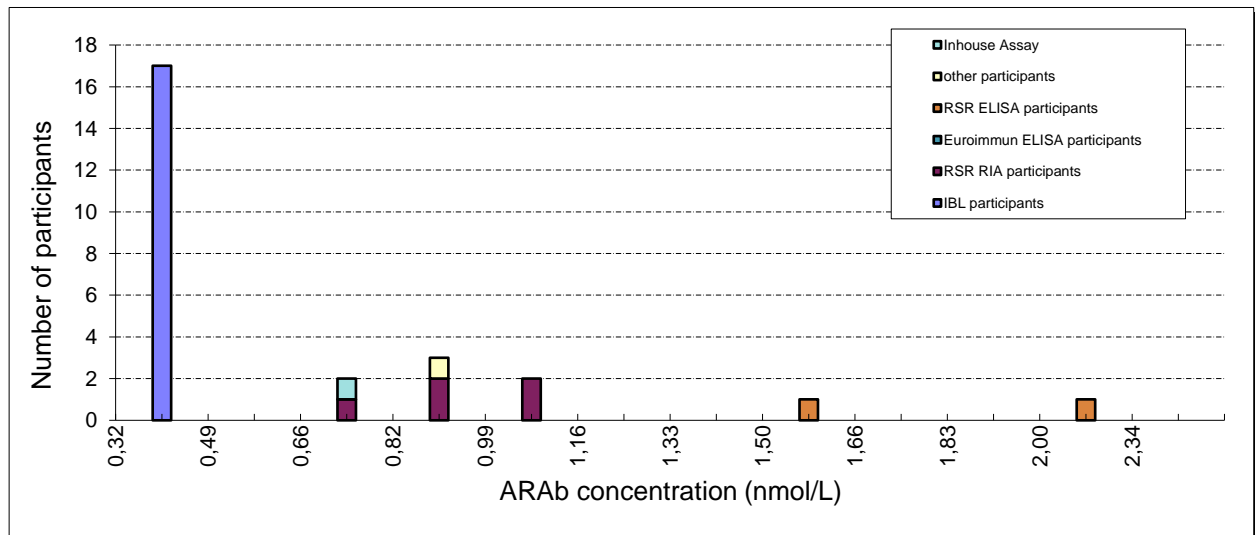

*The graphic is for information purposes only and not validated. Please read your results from the table.