

Quality Assessment Scheme for Acetylcholine receptor autoantibodies

The results from all participants can be found in the outstanding table, listed according to their Lab Number.


Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Cut-off		>0.4	≥0.5	≥0.5	≥0.45	≥0.5	none
Number of lab.		(nmol/L)	(nmol/L)	(nmol/L)	(nmol/L)	(nmol/L)	(nmol/L)
131	1,81	1,81					
199	2,47	2,47					
242	3,46		3,46				
364	3,29	3,29					
379	2,7	2,7					
381	2,73	2,73					
382	2,9						2,9
385	5,0		5,0				
389	2,13	2,13					
393	1,88	1,88					
397	1,44	1,44					
398	1,3	1,3					
399	1,75	1,75					
401	7,51				7,51		
402	1,82	1,82					
403	3,73	3,73					
406	2,3	2,3					
412	1,64	1,64					
414	2,28	2,28					
419	2,02	2,02					
421	3,48					3,48	
423	3,8					3,8	
425	2,7	2,7					
428	8,0				8,0		

Statistical Results Sample Number 24-2A:

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Mean	3,06	2,23	4,23	-	7,76	3,64	2,90
SD	1,71	0,65	1,09	-	0,35	0,23	-
Mean - 2SD	<0	0,94	2,05	-	7,06	3,19	-
Mean + 2SD	6,47	3,53	6,41	-	8,45	4,09	-
Amount	24	17	2	0	2	2	1


Samples have been determined by the single collectives as described below:

IBL	
Negative	< 0.25 nmol/L
Positive	> 0.40 nmol/L
Equivocal	0.25 – 0.40 nmol/L

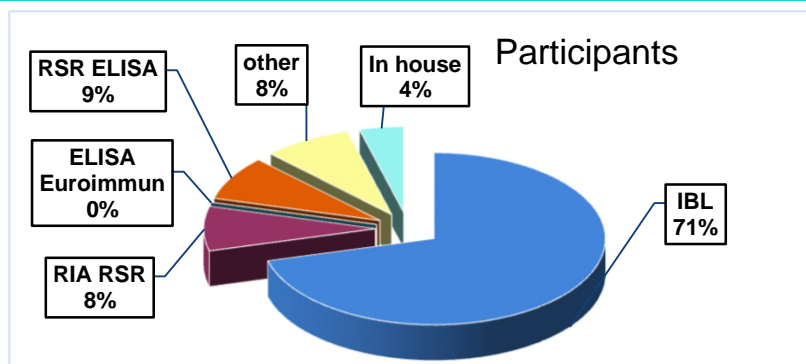

*The graphic is for information purposes only and not validated. Please read your results from the table.

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Negative	0	-	-	-	-	-	-
Equivocal	0	-	-	-	-	-	-
Positive	24	17	2	-	2	2	1
Amount	24	17	2	0	2	2	1

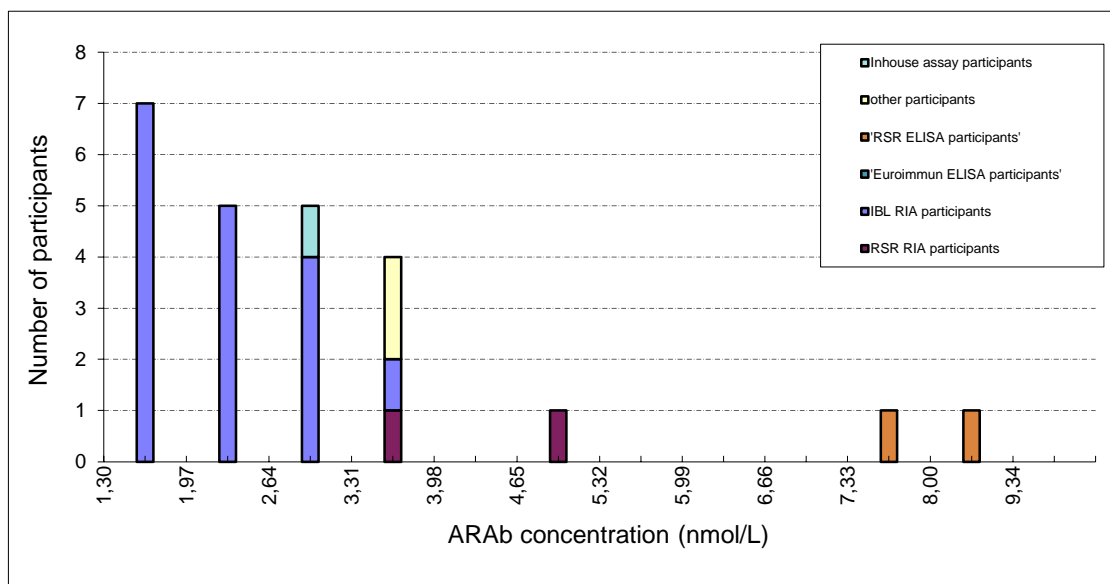

*The graphic is for information purposes only and not validated. Please read your results from the table.

The results from all participants can be found in the outstanding table, listed according to their Lab Number.


Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Cut-off		>0.4	≥0.5	≥0.5	≥0.45	≥0.5	none
Number of lab.		(nmol/L)	(nmol/L)	(nmol/L)	(nmol/L)	(nmol/L)	(nmol/L)
131	0,018	0,02					
199	0,12	0,12					
242	0,25		0,25				
364	0,25	0,25					
379	0,07	0,07					
381	0,02	0,02					
382	0						0,00
385	0,3		0,30				
389	0	0,00					
393	0	0,00					
397	0,2	0,20					
398	0,25	0,25					
399	0,1	0,10					
401	0,45				0,45		
402	0,03	0,03					
403	0,2	0,20					
406	0,25	0,25					
412	0,25	0,25					
414	0,2	0,20					
419	0	0,00					
421	0,1					0,10	
423	0,1					0,10	
425	0,25	0,25					
428	0,13				0,13		

Statistical Results Sample Number 24-2B:

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Mean	0,15	0,13	0,28	-	0,29	0,10	0,00
SD	0,12	0,11	0,04	-	0,23	0,00	-
Mean - 2SD	<0	<0	0,20	-	<0	0,10	-
Mean + 2SD	0,39	0,34	0,35	-	0,74	0,10	-
Amount	24	17	2	0	2	2	1


Samples have been determined by the single collectives as described below:

Negative < 0.25 nmol/L
 Positive > 0.40 nmol/L
 Equivocal 0.25 – 0.40 nmol/L

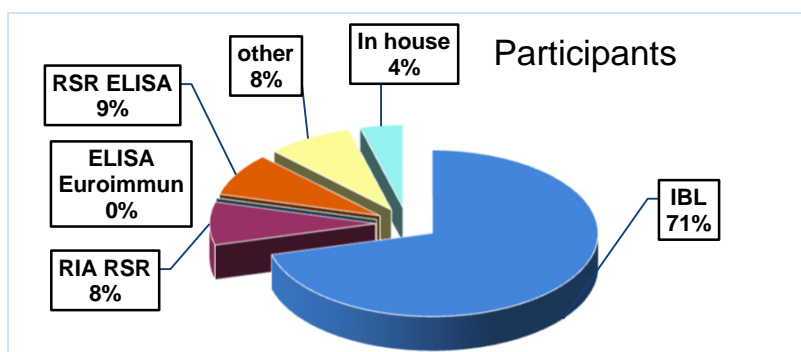

*The graphic is for information purposes only and not validated. Please read your results from the table.

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Negative	24	17	2	-	2	2	1
Equivocal	0	-	-	-	-	-	-
Positive	0	-	-	-	-	-	-
Amount	24	17	2	0	2	2	1

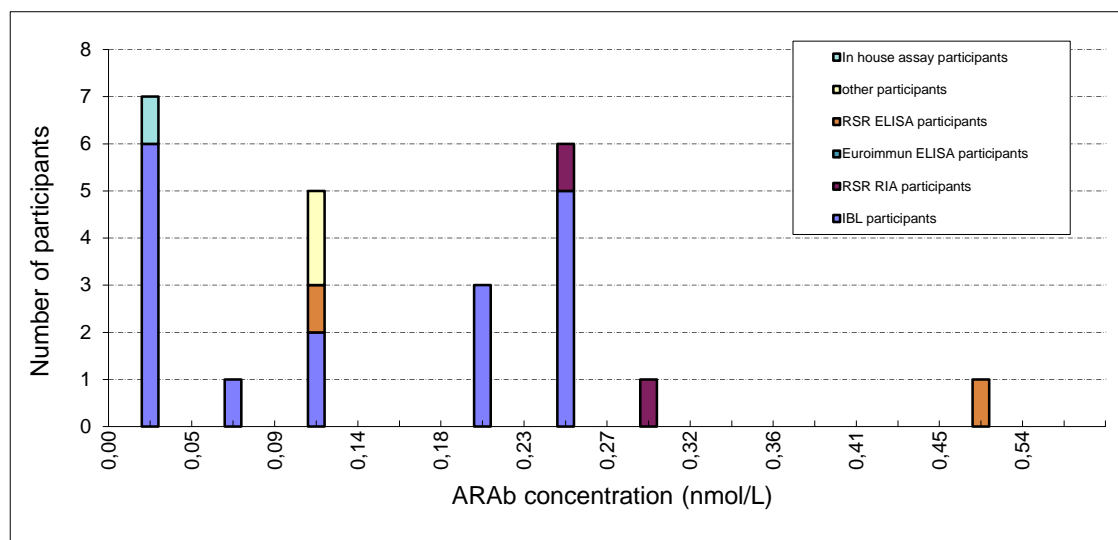

*The graphic is for information purposes only and not validated. Please read your results from the table.

The results from all participants can be found in the outstanding table, listed according to their Lab Number.


Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Cut-off		>0.4	≥0.5	≥0.5	≥0.45	≥0.5	none
Number of lab.		(nmol/L)	(nmol/L)	(nmol/L)	(nmol/L)	(nmol/L)	(nmol/L)
131	0,31	0,31					
199	0,36	0,36					
242	0,76		0,76				
364	0,30	0,30					
379	0,40	0,40					
381	0,35	0,35					
382	0,20						0,20
385	1,00		1,00				
389	0,32	0,32					
393	0,40	0,40					
397	0,29	0,29					
398	0,33	0,33					
399	0,36	0,36					
401	1,08				1,08		
402	0,29	0,29					
403	0,36	0,36					
406	0,34	0,34					
412	0,37	0,37					
414	0,41	0,41					
419	0,34	0,34					
421	0,92					0,92	
423	0,70					0,70	
425	0,40	0,40					
428	2,60				2,60		

Statistical Results Sample Number 24-2C:

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Mean	0,55	0,35	0,88	-	1,84	0,81	0,20
SD	0,50	0,04	0,17	-	1,07	0,16	-
Mean - 2SD	<0	0,27	0,54	-	<0	0,50	-
Mean + 2SD	1,55	0,43	1,22	-	3,99	1,12	-
Amount	24	17	2	0	2	2	1


Samples have been determined by the single collectives as described below:

Negative < 0.25 nmol/L
 Positive > 0.40 nmol/L
 Equivocal 0.25 – 0.40 nmol/L

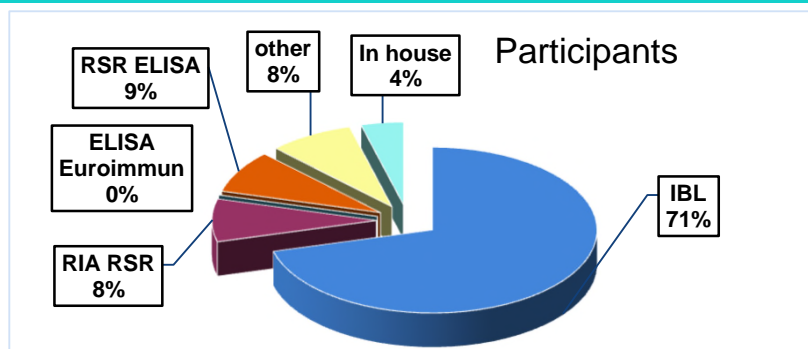

*The graphic is for information purposes only and not validated. Please read your results from the table.

Method	all	commercial kits					In house assay
		IBL	RSR RIA	ELISA Euroimmun	RSR ELISA	other	
Negative	1	-	-	-	-	-	1
Equivocal	20	17	1	-	2	-	-
Positive	3	-	1	-	-	2	-
Amount	24	17	2	0	2	2	1

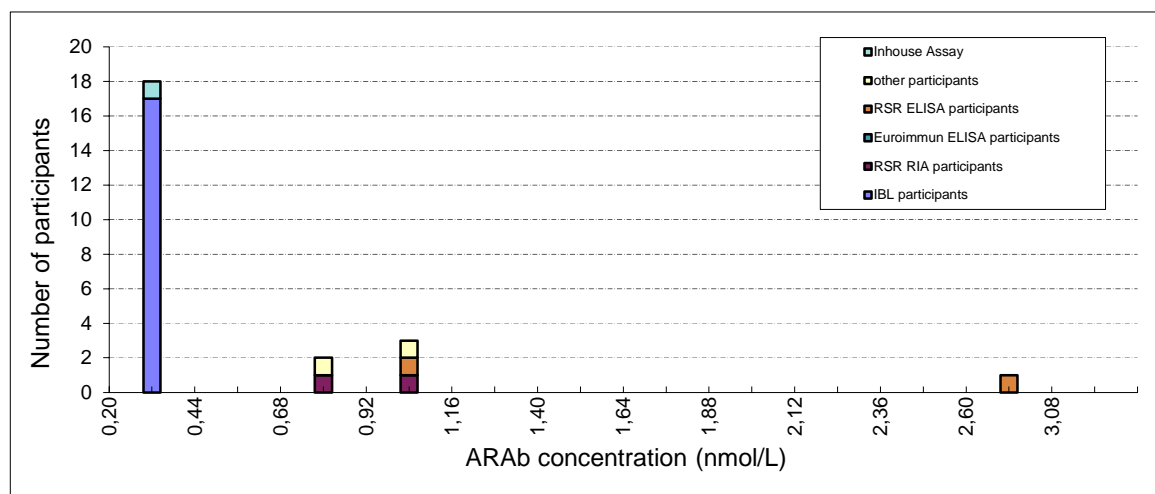

*The graphic is for information purposes only and not validated. Please read your results from the table.