

Quality Assessment Scheme for Salivary Steroids

Testosterone Sample Number 23-21


Your result: The results from all participants can be found in the outstanding table.

Method		LUM	ELISA		MS	
Supplier	all	IBL	IBL	Demeditec	DRG	In-House
Lab. Code	pg/mL	pg/mL	pg/mL	pg/mL	pg/mL	pg/mL
3013	5,520	5,52				
3019-1	9,464					9,46
3020	3,470					3,47
3030	2,776					2,78
3032	2,429					2,43
3036	7,886				7,89	
3047	3,249					3,25
3060			[2,157]			
3061	8,800		8,80			
13003	19,498		19,50			
13004	5,100	5,10				
15033	3,400					3,40
20002	19,080		19,08			
22236	5,681	5,68				
30001	4,984	4,98				
40001	7,800	7,80				
40002	5,710	5,71				
40003-1	9,970					9,97
40003-2	9,360		9,36			
40003-3	4,910	4,91				
40013	9,250				9,25	
40014	3,000					3,00
40015	18,100			18,10		
40016	22,400			22,40		
40024	4,000	4,00				
40027	16,520		16,52			
40029	18,700			18,70		
40036	12,210		12,21			
40041	26,100			26,10		
40049	15,840		15,84			
40054	26,000		26,00			
40055	14,800		14,80			

Statistical Results

Method		LUM	ELISA		MS	
Supplier	all	IBL	IBL	Demeditec	DRG	In-House
Mean	10,516	5,463	15,79	21,33	8,568	4,720
SD	7,187	1,094	5,401	3,708	0,964	3,106
Mean - 2SD	0,000	3,275	4,988	13,909	6,640	0,000
Mean + 2SD	24,891	7,652	26,592	28,741	10,497	10,931
Amount	31	8	9	4	2	8

*The graphic is for information purposes only and not validated. Please read your results from the table.

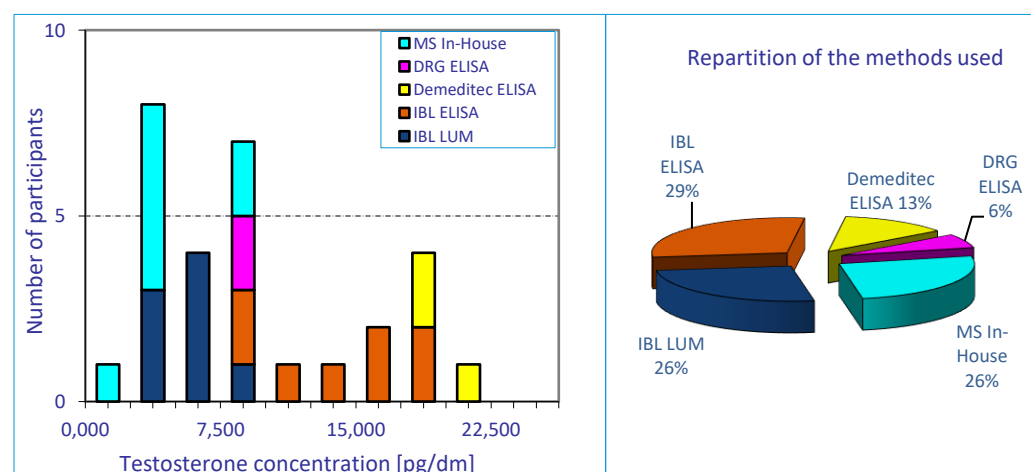

Quality Assessment Scheme for Salivary Steroids

Testosterone Sample Number 23-22


Your result: The results from all participants can be found in the outstanding table.

Method		LUM	ELISA		MS	
Supplier	all	IBL	IBL	Demeditec	DRG	In-House
Lab. Code	pg/mL	pg/mL	pg/mL	pg/mL	pg/mL	pg/mL
3013	31,41	31,41				
3019-1	37,54					37,54
3020	40,06					40,06
3030	35,49					35,49
3032	31,86					31,86
3036	29,24				29,24	
3047	37,85					37,85
3060	19,72		19,72			
3061	37,60		37,60			
6005	47,09		47,09			
13004	28,90	28,90				
15033	39,50					39,50
20002	48,22		48,22			
22236	32,58	32,58				
30001	28,86	28,86				
40001	34,80	34,80				
40002	34,95	34,95				
40003-1	56,71					56,71
40003-2	31,91		31,91			
40003-3	30,33	30,33				
40013	34,35				34,35	
40014	38,00					38,00
40015	54,50			54,50		
40016	51,40			51,40		
40024	27,00	27,00				
40027	53,84		53,84			
40029	52,92			52,92		
40036	34,50		34,50			
40041	64,50			64,50		
40049	57,50		57,50			
40054	43,00		43,00			
40055	37,60		37,60			

Statistical Results

Method		LUM	ELISA		MS	
Supplier	all	IBL	IBL	Demeditec	DRG	In-House
Mean	39,49	31,10	41,10	55,83	31,80	39,63
SD	10,57	2,88	11,21	5,92	3,61	7,36
Mean - 2SD	18,36	25,35	18,68	44,00	24,57	24,90
Mean + 2SD	60,63	36,86	63,52	67,66	39,02	54,36
Amount	32	8	10	4	2	8

*The graphic is for information purposes only and not validated. Please read your results from the table.

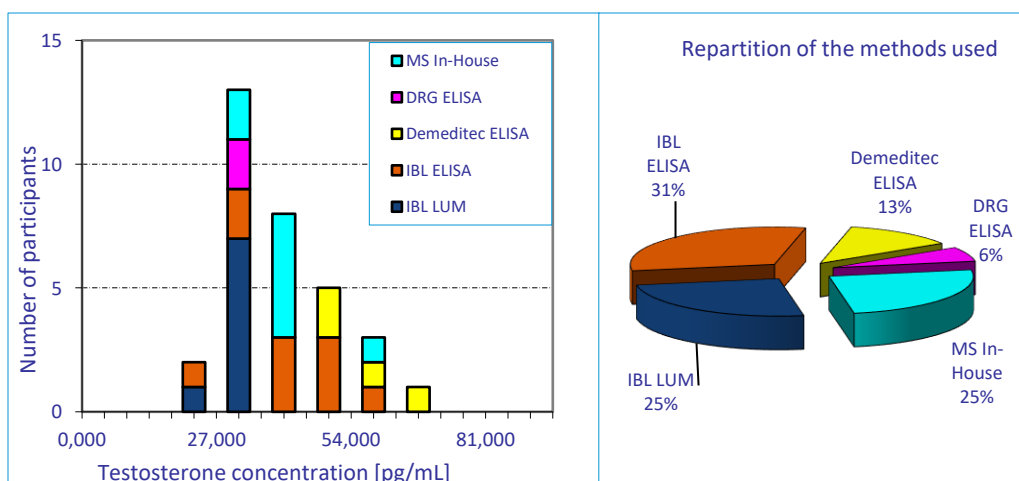

Quality Assessment Scheme for Salivary Steroids

Testosterone Sample Number 23-23

Your result: The results from all participants can be found in the outstanding table.

Method		LUM	ELISA		MS	
Supplier	all	IBL	IBL	Demeditec	DRG	In-House
Lab. Code	pg/mL	pg/mL	pg/mL	pg/mL	pg/mL	pg/mL
3013	109,8	109,8				
3019-1	106,7					106,7
3020	111,0					111,0
3030	109,9					109,9
3032	90,5					90,5
3036	72,5				72,5	
3047	123,7					123,7
3060	113,9		113,9			
3061	102,5		102,5			
6005	114,9		114,9			
13004	96,7	96,7				
15033	102,1					102,1
20002	140,4		140,4			
22236	112,0	112,0				
30001	122,4	122,4				
40001	98,5	98,5				
40002	102,6	102,6				
40003-1	156,8					156,8
40003-2	105,0		105,0			
40003-3	97,1	97,1				
40013	90,4				90,4	
40014	126,0					126,0
40015	121,0			121,0		
40016	113,5			113,5		
40024	96,0	96,0				
40027	160,0		160,0			
40029	118,7			118,7		
40036	120,5		120,5			
40041	132,9			132,9		
40049			[5,043]			
40054	131,0		131,0			
40055	95,9		95,9			

Statistical Results

Method		LUM	ELISA		MS	
Supplier	all	IBL	IBL	Demeditec	DRG	In-House
Mean	112,74	104,38	120,45	121,51	81,47	115,84
SD	18,75	9,50	20,34	8,21	12,65	20,05
Mean - 2SD	75,23	85,38	79,78	105,09	56,16	75,75
Mean + 2SD	150,24	123,38	161,12	137,94	106,78	155,93
Amount	31	8	9	4	2	8

*The graphic is for information purposes only and not validated. Please read your results from the table.

