

# Quality Control Certificate



## sInterleukin-2-Receptor ELISA


<b>REF</b> 30201813	<b>LOT</b> EIS128	<b>2026-06-30</b> YYYY-MM-DD
---------------------	-------------------	---------------------------------

**Final Release Results:**

	Concentration U/mL	Measured value OD	Range OD	OD/ODmax	e.g. automated*
					DSX Measured value OD
CAL A	0	0.017	-	1%	0.001
CAL B	7.0	0.205	-	8%	0.202
CAL C	20.0	0.603	-	25%	0.624
CAL D	40.0	1.126	-	47%	1.139
CAL E	80.0	1.900	-	79%	1.889
CAL F	160.0	2.414	-	100%	2.780

\*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

	Concentration found U/mL	Acceptable range		
		lower limit U/mL	target U/mL	upper limit U/mL
CONTROL 1	16	11	16	22
CONTROL 2	61	42	63	85

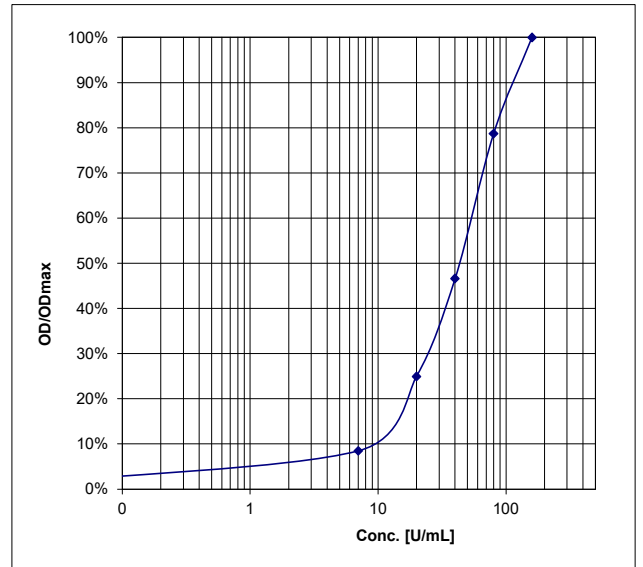

**Kit Composition:**

REF		LOT	
30201806	MTP	K233	2027-01
30201807	CAL A-F	K425	2027-06
30201808	CONTROL 1	K426	2027-06
30201809	CONTROL 2	K427	2027-06
30201810	BIOTIN AB	K428	2027-05
30201811	SAMPLEDIL	K440	2027-05
30201812	ENZCONJ	K429	2027-05
KIZZ01	CONC WASHBUF	K459	2029-04
KEZZ991	TMB SUBS	K132-7	2028-09
KIZZ71	TMB STOP	L912	2028-02

Valid edition of the instructions for use: 2025-02

**This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.**

Verified by: **Dr. Spangenberg**

Validation date: **2025-12-17**

**Accepted**

This document has been produced electronically and is valid without a signature.