

Quality Control Certificate



Interleukin-2-Receptor ELISA

REF 30201813

LOT EIS149


2027-09-30
YYYY-MM-DD

Final Release Results:

<u><u>Final Release Results:</u></u>					e.g. automated*
	Concentration	Measured value	Range	OD/ODmax	DSX Measured value
	U/mL	OD	OD		OD
CAL A	0	0.020	-	1%	0.007
CAL B	6.0	0.123	-	7%	0.133
CAL C	20.0	0.346	-	19%	0.367
CAL D	40.0	0.720	-	41%	0.755
CAL E	80.0	1.207	-	68%	1.388
CAL F	160.0	1.777	-	100%	2.231

*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

	Concentration found U/mL	Acceptable range		
		lower limit U/mL	target U/mL	upper limit U/mL
CONTROL 1	17	10	15	21
CONTROL 2	58	43	66	88

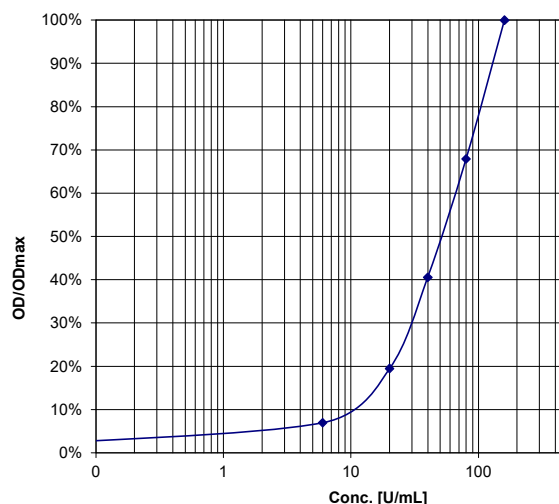

Kit Composition:

REF		LOT	
30201806	MTP	K718	2027-11
30201807	CAL A-F	K893	2027-12
30201808	CONTROL 1	K894	2027-12
30201809	CONTROL 2	K895	2027-12
30201810	BIOTIN AB	K597	2027-09
30201811	SAMPLEDIL	K594	2028-02
30201812	ENZCONJ	K907	2028-02
K1ZZZ01	CONC WASHBUF	K596	2029-08
KEZZ991	TMB SUBS	K503-3	2029-04
K1ZZZ71	TMB STOP	K698	2029-03

Valid edition of the instructions for use:

2026-03

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: T. Borchert

Validation date: 2026-09-16

Accepted

This document has been produced electronically and is valid without a signature.



IBL International GmbH
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11
E-MAIL: ibl@tecan.com
WEB: www.tecan.com/ibl