

# Quality Control Certificate



## DHEA ELISA


|                     |                    |                                 |
|---------------------|--------------------|---------------------------------|
| <b>REF</b> 30252873 | <b>LOT</b> EDH131U | <b>2026-07-31</b><br>YYYY-MM-DD |
|---------------------|--------------------|---------------------------------|

**Final Release Results:**

|       | Concentration<br>ng/mL | manual               |         |          | e.g.automated/DSX    |
|-------|------------------------|----------------------|---------|----------|----------------------|
|       |                        | Measured value<br>OD | Range*  | OD/ODmax | Measured value<br>OD |
| CAL A | 0.0                    | 1.980                | > 1.000 | 100%     | 2.219                |
| CAL B | 0.37                   | 1.554                | -       | 78%      | 1.791                |
| CAL C | 1.10                   | 1.088                | -       | 55%      | 1.294                |
| CAL D | 3.30                   | 0.662                | -       | 33%      | 0.831                |
| CAL E | 10.0                   | 0.344                | -       | 17%      | 0.448                |
| CAL F | 30.0                   | 0.168                | -       | 8%       | 0.220                |

\*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

| Validation criteria |                              |                      |                 |                      |
|---------------------|------------------------------|----------------------|-----------------|----------------------|
|                     | Concentration found<br>ng/mL | Acceptable range     |                 |                      |
|                     |                              | lower limit<br>ng/mL | target<br>ng/mL | upper limit<br>ng/mL |
| CONTROL 1           | 1.9                          | 1.1                  | 1.8             | 2.6                  |
| CONTROL 2           | 5.1                          | 4.0                  | 5.0             | 6.0                  |

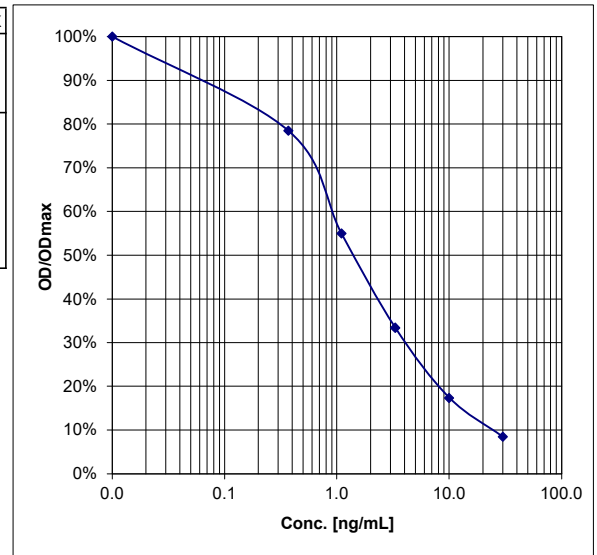

**Kit Composition:**

| REF     |              | LOT    |         |
|---------|--------------|--------|---------|
| KEDH511 | MTP          | L559   | 2026-07 |
| KEDH541 | ENZCONJ      | L580   | 2026-08 |
| KEDH611 | CAL A-F      | L577   | 2026-07 |
| KEDH651 | CONTROL 1    | L578   | 2026-07 |
| KEDH661 | CONTROL 2    | L579   | 2026-07 |
| KEZZ991 | TMB SUBS     | L541-2 | 2027-10 |
| KEZZ921 | TMB STOP     | L553   | 2027-08 |
| KIZZ01  | CONC WASHBUF | L554   | 2028-03 |

| REF | LOT |  |
|-----|-----|--|
|     |     |  |

Valid edition of the instructions for use: 2025-03

**This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.**

Verified by: M.Dries

Validation date: 2025-05-27

**Accepted**

This document has been produced electronically and is valid without a signature.