

Quality Control Certificate




Androstane-diol- Glucuronide ELISA

REF	DB52171	LOT	261500	2027-07-31 YYYY-MM-DD
------------	----------------	------------	---------------	---------------------------------

Final Release Results:

	Concentration ng/mL	Measured value OD	Range OD	OD/ODmax
CAL A	0	2.766	> 2.000	100%
CAL B	0.25	1.910	-	69%
CAL C	1	1.167	-	42%
CAL D	3	0.705	-	25%
CAL E	10	0.336	-	12%
CAL F	50	0.121	-	4%

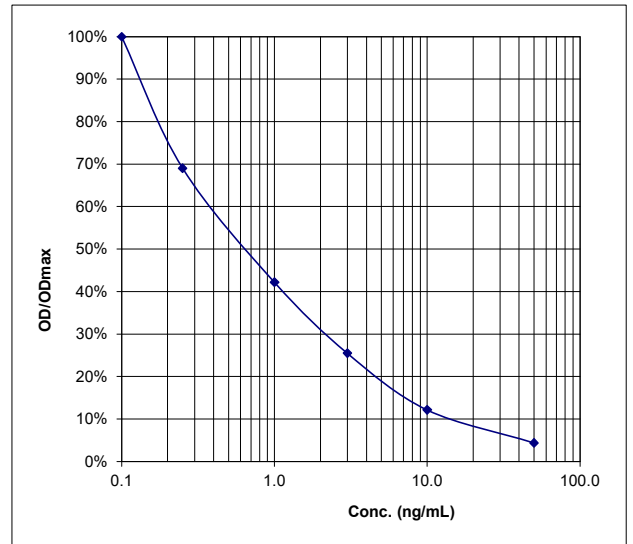

	Result	Acceptable Range
OD Standard F/% Binding	0.121/4%	< 12%

	Concentration found ng/mL	Target Value ng/mL	Acceptable range lower limit ng/mL	upper limit ng/mL
KIT CONTROL High CS3921	8.06	8.09	6.07	10.11
KIT CONTROL Low CS3921	1.62	1.69	1.27	2.11

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: Dr. Spangenberg

Validation date: 2026-05-07

Accepted

This document has been produced electronically and is valid without a signature.



IBL International GmbH
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11
E-MAIL: ibl@tecan.com
WEB: www.tecan.com/ibl