

Quality Control Certificate



Free Testosteron(e) ELISA


REF DB52181	LOT EFT142	2026-05-31 YYYY-MM-DD
--------------------	-------------------	---------------------------------

Final Release Results:

	Concentration pg/mL	manual			e.g. automated/ DSX
		Measured value OD	Range*	OD/ODmax	Measured value OD
CAL A	0	2.226	-	100%	1.639
CAL B	0.25	2.083	-	94%	1.555
CAL C	2.5	1.605	-	72%	1.294
CAL D	10	1.053	-	47%	0.878
CAL E	25	0.619	-	28%	0.496
CAL F	100	0.156	-	7%	0.129

*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

Validation criteria (manual/automated)				
	Concentration found pg/mL	Acceptable range		
		lower limit pg/mL	target value pg/mL	upper limit pg/mL
CONTROL 1	2.4	1.3	2.2	3.1
CONTROL 2	19.8	13.7	19.6	25.5

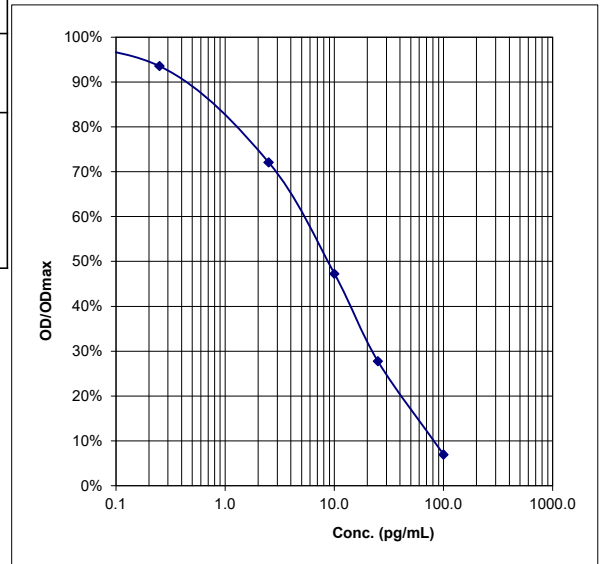

Kit Composition:

REF		LOT	
KEFT511	MTP	L710	2026-10
KEFT541	ENZCONJ	L726	2026-06
KEFT611	CAL A-F	L722	2026-05
KEFT651	CONTROL 1	L723	2026-05
KEFT661	CONTROL 2	L724	2026-05
KIZZ01	CONC WASHBUF	L686	2028-04
KEZZ991	TMB SUBS	L704	2027-10
KEZZ921	TMB STOP	L705	2027-11

REF	LOT	

Valid edition of the instructions for use: 2023-11

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: M.Dries

Validation date: 2024-12-10

Accepted

This document has been produced electronically and is valid without a signature.