

Quality Control Certificate



IgA Saliva ELISA

REF DM59171


LOT 6643A

2027-09-30
YYYY-MM-DD

Final Release Results:

	Calibrator concentration µg/mL	Measured value OD	Range OD	OD/ODmax
CAL 0	0	0.043	-	2%
CAL 1	6.9	0.165	> 0.065	7%
CAL 2	62	0.826	> 0.330	35%
CAL 3	132	1.364	> 0.545	58%
CAL 4	400	2.350	> 0.940	100%

	Concentration found µg/mL	Acceptable range		
		lower limit µg/mL	target µg/mL	upper limit µg/mL
CONTROL	86.8	54.6	84.0	113.4

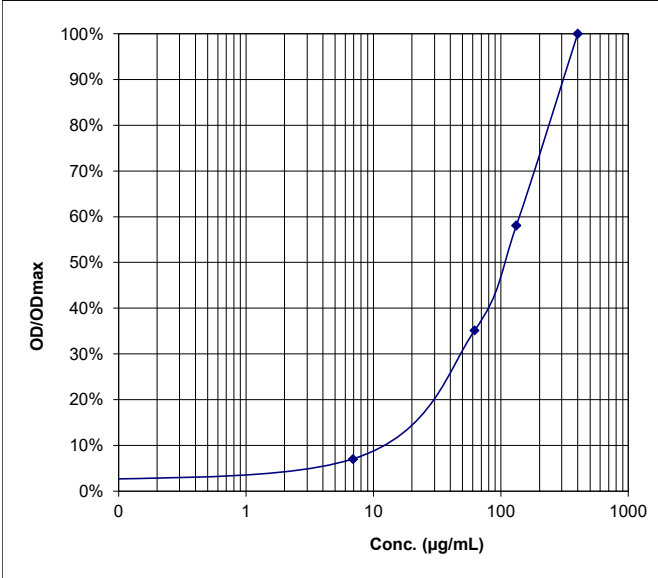

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: Dr. Spangenberg

Validation date: 2026-07-29

Accepted

This document has been produced electronically and is valid without a signature.



IBL International GmbH
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11
E-MAIL: ibl@tecan.com
WEB: www.tecan.com/ibl