

Quality Control Certificate




IgA Saliva ELISA

REF	DM59171	LOT	6664A		2027-11-30
					YYYY-MM-DD

Final Release Results:

	Calibrator concentration µg/mL	Measured value OD	Range OD	OD/ODmax
CAL 0	0	0.089	-	4%
CAL 1	6.9	0.207	> 0.085	9%
CAL 2	62	0.950	> 0.380	39%
CAL 3	132	1.416	> 0.565	59%
CAL 4	400	2.419	> 0.970	100%

	Concentration found µg/mL	Acceptable range		
		lower limit µg/mL	target µg/mL	upper limit µg/mL
CONTROL	82.81	53.23	81.90	110.56

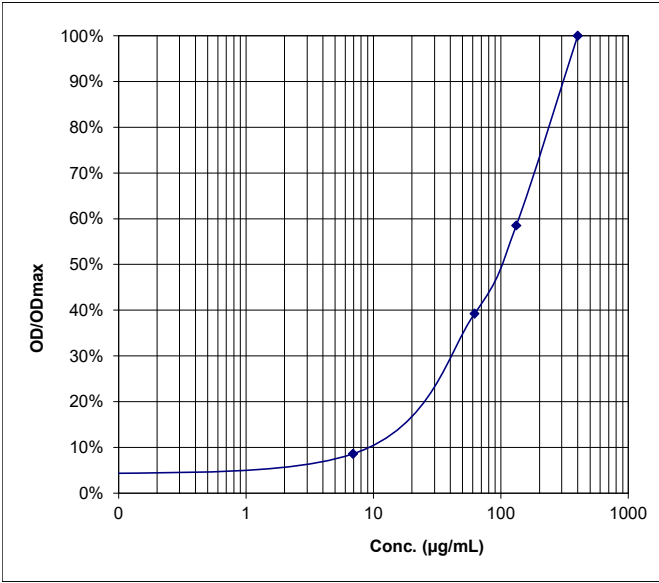

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: Dr. Spangenberg

Validation date: 2026-09-18

Accepted

This document has been produced electronically and is valid without a signature.



IBL International GmbH
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11
E-MAIL: ibl@tecan.com
WEB: www.tecan.com/ibl