Quality Control Certificate

dsDNA-Ab RIA

REF RE19011	LOT RDD389	2027-01-28 YYYY-MM-DD

Final Release Results:

		Measured value	
Total Activitiy	TA	22623	cpm
Non-specific binding/TA	NSB/TA	2.8	%
Maximum Binding/TA	(Bmax-NSB)/TA	56	%

	Concentration IU/mL	Measured value cpm	Range cpm	(B-NSB) / (Bmax-NSB)
CAL A	0	627	-	0%
CAL B	4.0	1144	-	4%
CAL C	7.0	1647	-	8%
CAL D	14	2960	-	19%
CAL E	40	6860	-	49%
CAL F	80	13235	-	100%

	Concentration found IU/mL	Acceptable range lower limit IU/mL	target value IU/mL	upper limit IU/mL
CONTROL 1	2.8	0.1	2.6	5.1
CONTROL 2	24.2	19.3	24.1	28.9

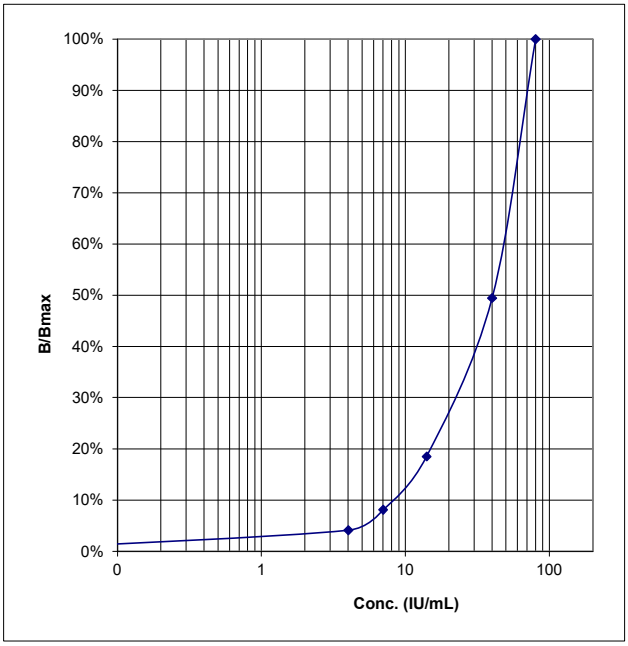

Kit Composition:

REF		LOT	
KRDD151	LYO CONTROL 1	H793-B	2027-04
KRDD161	LYO CONTROL 2	H794-B	2027-04
KRDD011	TRACER	H872	2027-01-28
KRDD111A-F	LYO CAL A-F	H782-B	2027-04
KRDD261	LYO SAMPLEDIL	H808-B	2027-04
KRDD051	AMMSULF	H747	2027-06

Valid edition of the instructions for use: 2022-11

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: Dr. Spangenberg

Validation date: 2026-11-02

Accepted

This document has been produced electronically and is valid without a signature.

IBL International GmbH
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11
E-MAIL: ibl@tecan.com
WEB: www.tecan.com/ibl