

Quality Control Certificate



Acetylcholine Receptor Autoantibodies (ARAb) RRA

REF RE21021 & RE21023

LOT RAR571


2026-11-24
YYYY-MM-DD

Final Release Results:

		Measured value	
Total Activity	TA	89503	cpm
Binding of Standard A	B0/TA	1.4	%
Maximum Binding	Bmax/TA	23	%

	Concentration	Measured value	Range	B/Bmax
	nmol/L	cpm	cpm	
CAL A	0	1255	-	0%
CAL B	0.2	2676	-	7%
CAL C	0.5	5324	-	20%
CAL D	1.2	11333	-	48%
CAL E	3	17865	-	80%
CAL F	8	22042	-	100%

	Concentration found	Acceptable range		
	nmol/L	lower limit	target value	upper limit
	nmol/L	nmol/L	nmol/L	nmol/L
CONTROL CO	0.44	0.34	0.43	0.51
CONTROL +	1.13	0.81	1.16	1.51

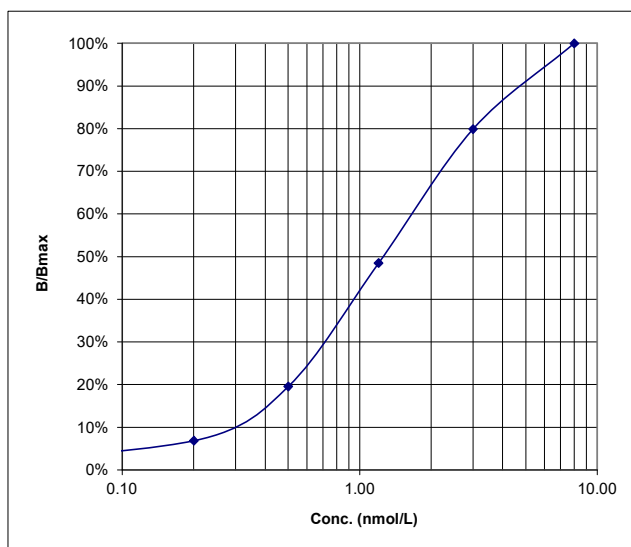

Kit Composition:

REF		LOT	
KRAR013	LYO TRACER	H817	2026-11-24
KRAR031/33	ANTISERUM	H715-C	2026-11
KRAR111A	CAL A	H450-8G	2026-11-24
KRAR111B-F	CAL B-F	H440-14M	2026-11-24
KRAR151	CONTROL CO	H441-14M	2026-11-24

REF		LOT	
KRAR161	CONTROL +	H442-14M	2026-11-24
KRAR253	WASHBUF	H772	2028-07
KRAR261	BUF	H743-B	2026-11

Valid edition of the instructions for use: 2023-08

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: T. Borchert

Validation date: 2026-09-02

Accepted

This document has been produced electronically and is valid without a signature.



IBL International GmbH
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11
E-MAIL: ibl@tecan.com
WEB: www.tecan.com/ibl