

Quality Control Certificate



Melatonin direct Serum/Plasma/Saliva RIA (Serum/Plasma)


REF RE29301	LOT RMD510	2026-06-11 YYYY-MM-DD
--------------------	-------------------	---------------------------------

Final Release Results:

		Measured value	
Total Activity	TA	92560	cpm
Non-specific binding/TA	NSB/TA	1.1	%
Maximum Binding/TA	(B0-NSB)/TA	24	%

	Concentration pg/mL	Measured value cpm	Range cpm	(B-NSB) / (B0-NSB)
NSB	-	971	-	-
CAL A	0	23347	-	100%
CAL B	2.5	22493	-	96%
CAL C	7.5	19897	-	85%
CAL D	25	14236	-	59%
CAL E	75	9582	-	38%
CAL F	250	5695	-	21%
CAL G	750	3624	-	12%

	Measured value pg/mL	Acceptable range		
		lower limit pg/mL	target value pg/mL	upper limit pg/mL
CONTROL 1	10	6	9	13
CONTROL 2	101	74	97	121

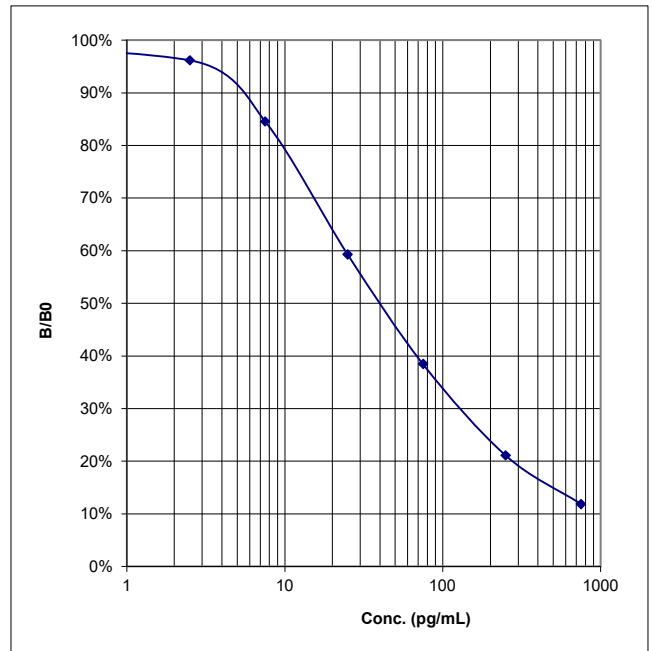

Kit Composition:

REF	LOT		REF	LOT			
KRMD151	CONTROL 1	H632	2027-02	KRMD251	ASSAYBUF	H605	2027-12
KRMD161	CONTROL 2	H633	2027-02	KRMD275	LYO ENZ	H634	2027-01
KRMD011	LYO TRACER	H673	2026-06-11	KRMD281	ENZBUF	H433	2026-11
KRMD035	LYO ANTISERUM	H297	2027-01				
KRMD051	PREC ANTISERUM	H639	2027-02				
KRMD111	CONC CAL A-G	H631	2027-02				
KRMD261	LYO DIL	H435	2028-06				

Valid edition of the instructions for use: V2020-02

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: S. Geweke

Validation date: 2026-03-17

Accepted

This document has been produced electronically and is valid without a signature.



IBL International GmbH
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11
E-MAIL: ibl@tecan.com
WEB: www.tecan.com/ibl