

# Quality Control Certificate



## 17-OH-Progesterone ELISA

REF RE52071


LOT EOH244

2026-07-31  
YYYY-MM-DD

### Final Release Results:

	Concentration ng/mL	Measured value OD	manual		e.g. automated DSX
			Range* OD	OD/ODmax	Measured value OD
CAL A	0	2.027	> 1.000	100%	1.664
CAL B	0.15	1.552	-	77%	1.239
CAL C	0.5	1.008	-	50%	0.789
CAL D	1.5	0.558	-	28%	0.435
CAL E	3.0	0.349	-	17%	0.260
CAL F	7.5	0.184	-	9%	0.134
CAL G	20	0.097	< 0.350	5%	0.067

\*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

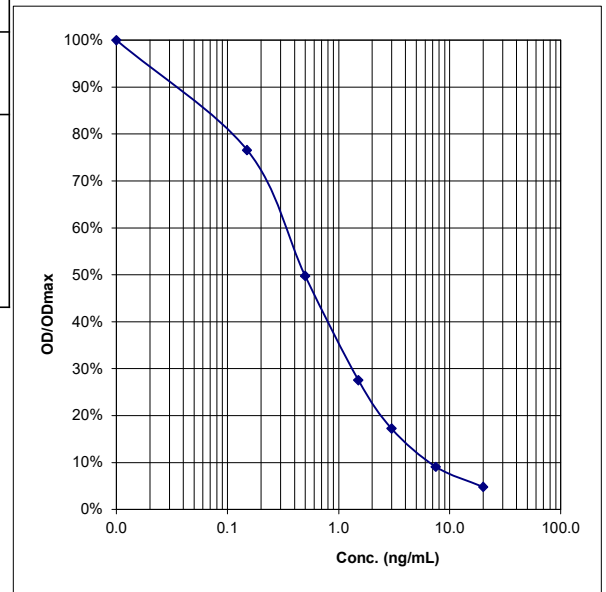

### Validation criteria

	Concentration found ng/mL	Acceptable range		
		lower limit ng/mL	target ng/mL	upper limit ng/mL
CONTROL 1	0.95	0.53	0.96	1.39
CONTROL 2	3.8	2.5	3.9	5.3

### Kit Composition:

REF		LOT	
KEOH651	CONTROL1	L677	2026-10
KEOH661	CONTROL2	L678	2026-10
KEOH511	MTP	L591	2028-04
KEOH541	ENZCONJ	L679	2026-10
KEOH611	CAL A	L676	2026-10
KEOH611	CAL B-G	L676	2026-10
KEZZ751	CONC WASHBUF	L419	2026-07
KEZZ991	TMB SUBS	L704-2	2027-10

REF		LOT	
KEZZ921	TMB STOP	L720	2027-11

Valid edition of the instructions for use: 2024-02

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: Dr. Spangenberg

Validation date: 2025-01-08

**Accepted**

This document has been produced electronically and is valid without a signature.



IBL International GmbH  
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11  
E-MAIL: [ibl@tecan.com](mailto:ibl@tecan.com)  
WEB: [www.tecan.com/ibl](http://www.tecan.com/ibl)