

# Quality Control Certificate



## DHEA-S ELISA


<b>REF</b> RE52181	<b>LOT</b> EDS138	<b>2027-02-28</b> YYYY-MM-DD
--------------------	-------------------	---------------------------------

### Final Release Results:

	Concentration µg/mL	Measured value OD	manual	
			Range*	OD/ODmax
CAL A	0	2.530	> 1.000	100%
CAL B	0.1	1.891	-	75%
CAL C	0.3	1.364	-	54%
CAL D	0.9	0.832	-	33%
CAL E	2.7	0.428	-	17%
CAL F	10.0	0.166	-	7%

\*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

Validation criteria				
	Concentration found µg/mL	Acceptable range		
		lower limit µg/mL	target µg/mL	upper limit µg/mL
CONTROL 1	0.51	0.33	0.51	0.68
CONTROL 2	2.5	2.1	2.6	3.1

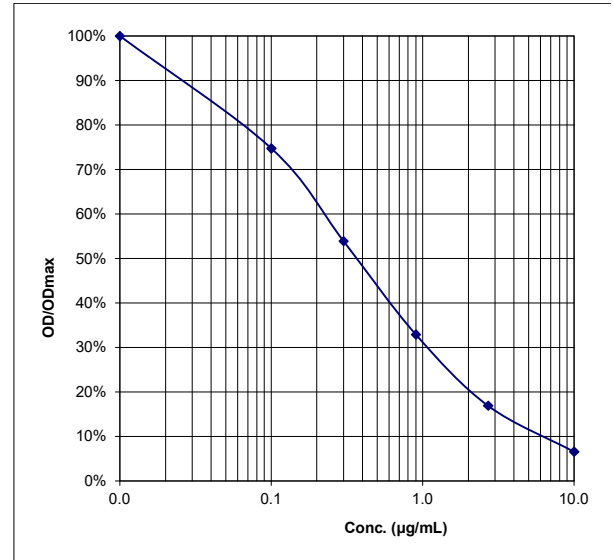

### Kit Composition:

REF		LOT	
KEDS651	CONTROL 1	L888	2027-04
KEDS661	CONTROL 2	L889	2027-04
KEDS511	MTP	L886	2027-08
KEDS541	ENZCONJ	L890	2027-04
KEDS611	CAL A	L887	2027-04
KEDS611	CAL B-F	L887	2027-04
KIZZ01	CONC WASHBUF	L862	2028-07
KEZZ991	TMB SUBS	M840-5	2027-02

REF		LOT	
KEZZ921	TMB STOP	L132	2027-02

Valid edition of the instructions for use: Version 2017-03

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: M.Dries

Validation date: 2025-03-17

# Accepted

This document has been produced electronically and is valid without a signature.



**IBL International GmbH**  
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11  
E-MAIL: [IBL@IBL-International.com](mailto:IBL@IBL-International.com)  
WEB: <http://www.IBL-International.com>