

# Quality Control Certificate



## DHEA-S ELISA


<b>REF</b> RE52181	<b>LOT</b> EDS139	<b>2028-01-31</b> YYYY-MM-DD
--------------------	-------------------	---------------------------------

### Final Release Results:

	Concentration µg/mL	Measured value OD	manual	
			Range*	OD/ODmax
CAL A	0	1.918	> 1.000	100%
CAL B	0.1	1.241	-	65%
CAL C	0.3	0.838	-	44%
CAL D	0.9	0.481	-	25%
CAL E	2.7	0.247	-	13%
CAL F	10.0	0.098	-	5%

\*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

Validation criteria				
	Concentration found µg/mL	Acceptable range		
		lower limit µg/mL	target µg/mL	upper limit µg/mL
CONTROL 1	0.51	0.34	0.52	0.70
CONTROL 2	2.4	2.0	2.5	3.0

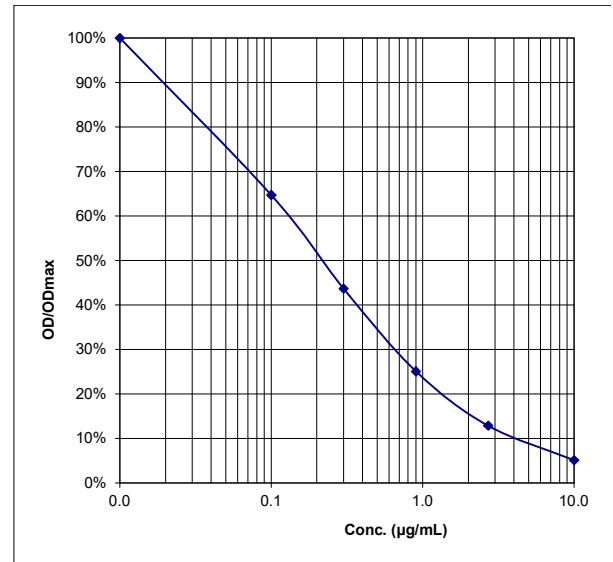

### Kit Composition:

REF		LOT	⌚
KEDS651	CONTROL 1	K518	2028-02
KEDS661	CONTROL 2	K519	2028-02
KEDS511	MTP	K277	2028-06
KEDS541	ENZCONJ	K516	2028-02
KEDS611	CAL A	K517	2028-02
KEDS611	CAL B-F	K517	2028-02
KIZZ01	CONC WASHBUF	K459	2029-04
KEZZ991	TMB SUBS	L919	2028-06

REF		LOT	⌚
KEZZ921	TMB STOP	K133	2028-05

Valid edition of the instructions for use: Version 2017-03

**This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.**

Verified by: T. Borchert

Validation date: 2026-01-14

# Accepted

This document has been produced electronically and is valid without a signature.



**IBL International GmbH**  
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11  
E-MAIL: [IBL@IBL-International.com](mailto:IBL@IBL-International.com)  
WEB: <http://www.IBL-International.com>