

# Quality Control Certificate



## DHEA ELISA


<b>REF</b> RE52221	<b>LOT</b> EDH131	<b>2026-07-31</b> YYYY-MM-DD
--------------------	-------------------	---------------------------------

### Final Release Results:

	Concentration ng/mL	manual			e.g.automated/DSX
		Measured value OD	Range*	OD/ODmax	Measured value OD
CAL A	0.0	1.980	> 1.000	100%	2.219
CAL B	0.37	1.554	-	78%	1.791
CAL C	1.10	1.088	-	55%	1.294
CAL D	3.30	0.662	-	33%	0.831
CAL E	10.0	0.344	-	17%	0.448
CAL F	30.0	0.168	-	8%	0.220

\*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

Validation criteria				
	Concentration found ng/mL	Acceptable range		
		lower limit ng/mL	target ng/mL	upper limit ng/mL
CONTROL 1	1.9	1.1	1.8	2.6
CONTROL 2	5.1	4.0	5.0	6.0

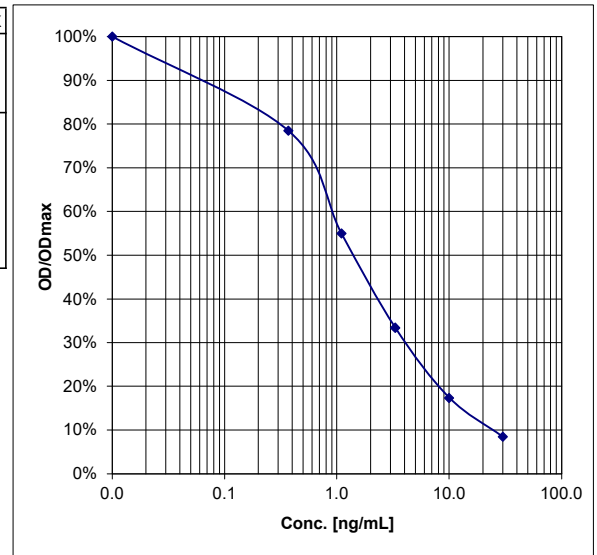

### Kit Composition:

REF		LOT	
KEDH511	MTP	L559	2026-07
KEDH541	ENZCONJ	L580	2026-08
KEDH611	CAL A-F	L577	2026-07
KEDH651	CONTROL 1	L578	2026-07
KEDH661	CONTROL 2	L579	2026-07
KEZZ991	TMB SUBS	L541-2	2027-10
KEZZ921	TMB STOP	L553	2027-08
KIZZ01	CONC WASHBUF	L554	2028-03

REF	LOT	

Valid edition of the instructions for use: 2023-09

**This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.**

Verified by: S. Geweke

Validation date: 2024-10-16

Accepted

This document has been produced electronically and is valid without a signature.



**IBL International GmbH**  
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11  
E-MAIL: [ibl@tecan.com](mailto:ibl@tecan.com)  
WEB: [www.tecan.com/ibl](http://www.tecan.com/ibl)