

Quality Control Certificate



DHEA ELISA


REF RE52221	LOT EDH132	2027-05-31 YYYY-MM-DD
--------------------	-------------------	---------------------------------

Final Release Results:

	Concentration ng/mL	manual			e.g.automated/DSX
		Measured value OD	Range* OD	OD/ODmax OD	Measured value OD
CAL A	0.0	2.175	> 1.000	100%	2.412
CAL B	0.37	1.664	-	77%	1.969
CAL C	1.10	1.167	-	54%	1.451
CAL D	3.30	0.722	-	33%	0.951
CAL E	10.0	0.375	-	17%	0.525
CAL F	30.0	0.191	-	9%	0.257

*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

Validation criteria				
	Concentration found ng/mL	Acceptable range		
		lower limit ng/mL	target ng/mL	upper limit ng/mL
CONTROL 1	2.1	1.2	2.0	2.8
CONTROL 2	5.2	4.0	5.0	6.0

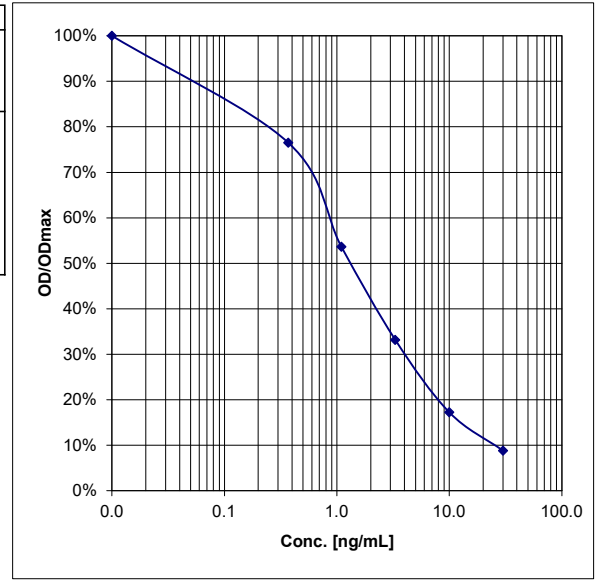

Kit Composition:

REF		LOT	⌚
KEDH511	MTP	K227	2027-05
KEDH541	ENZCONJ	K237	2027-05
KEDH611	CAL A-F	K234	2027-05
KEDH651	CONTROL 1	K235	2027-05
KEDH661	CONTROL 2	K236	2027-05
KEZZ991	TMB SUBS	K132-2	2028-09
KEZZ921	TMB STOP	L458	2027-07
KIZZ01	CONC WASHBUF	L862	2028-07

REF	LOT	⌚

Valid edition of the instructions for use: 2025-03

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: **Dr. Spangenberg**

Validation date: **2025-07-02**

Accepted

This document has been produced electronically and is valid without a signature.



IBL International GmbH
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11
E-MAIL: ibl@tecan.com
WEB: www.tecan.com/ibl