

# Quality Control Certificate



## DHEA ELISA


<b>REF</b> RE52221	<b>LOT</b> EDH133	<b>2027-09-30</b> YYYY-MM-DD
--------------------	-------------------	---------------------------------

**Final Release Results:**

	Concentration ng/mL	manual			e.g.automated/DSX
		Measured value OD	Range* OD	OD/ODmax OD	Measured value OD
CAL A	0.0	2.323	> 1.000	100%	1.971
CAL B	0.37	1.627	-	70%	1.532
CAL C	1.10	1.217	-	52%	1.073
CAL D	3.30	0.739	-	32%	0.667
CAL E	10.0	0.451	-	19%	0.396
CAL F	30.0	0.202	-	9%	0.175

\*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

Validation criteria				
	Concentration found ng/mL	Acceptable range		
		lower limit ng/mL	target ng/mL	upper limit ng/mL
CONTROL 1	1.7	1.1	1.8	2.5
CONTROL 2	5.8	4.4	5.5	6.6

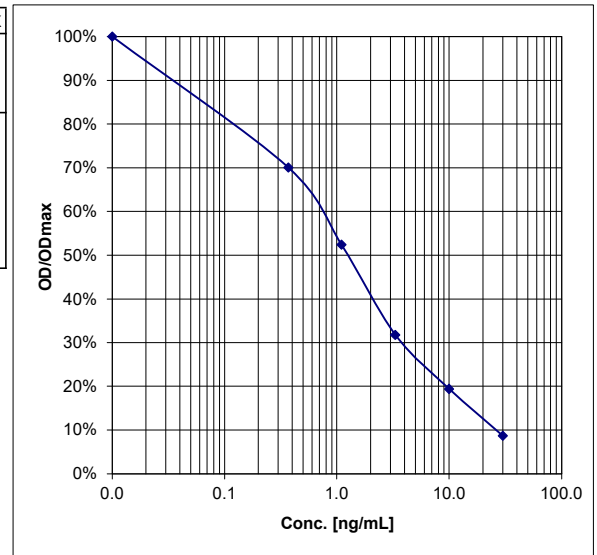

**Kit Composition:**

REF		LOT	
KEDH511	MTP	K430	2027-09
KEDH541	ENZCONJ	K434	2027-10
KEDH611	CAL A-F	K431	2027-10
KEDH651	CONTROL 1	K432	2027-10
KEDH661	CONTROL 2	K433	2027-10
KEZZ991	TMB SUBS	K132-7	2028-09
KEZZ921	TMB STOP	K441	2028-11
KIZZ01	CONC WASHBUF	K477	2029-05

REF	LOT	

Valid edition of the instructions for use: 2025-03

**This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.**

Verified by: T. Borchert

Validation date: 2025-12-17

**Accepted**

This document has been produced electronically and is valid without a signature.