

Quality Control Certificate



Progesterone Saliva ELISA


REF RE52281	LOT EPR144	2027-06-30 YYYY-MM-DD
--------------------	-------------------	---------------------------------

Final Release Results:

	Concentration pg/mL	manual			e.g. automated EVOlyzer
		Measured value OD	Range* OD	OD/ODmax OD	Measured value OD
CAL A	0	2.134	> 1.000	100%	2.044
CAL B	25	1.677	-	79%	1.731
CAL C	50	1.475	-	69%	1.504
CAL D	250	0.867	-	41%	0.912
CAL E	1000	0.354	-	17%	0.360
CAL F	5000	0.082	-	4%	0.088

*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

Validation criteria				
	Concentration found pg/mL	Acceptable range		
		lower limit pg/mL	target pg/mL	upper limit pg/mL
CONTROL 1	56.8	42.8	61.1	79.5
CONTROL 2	617	440	628	817

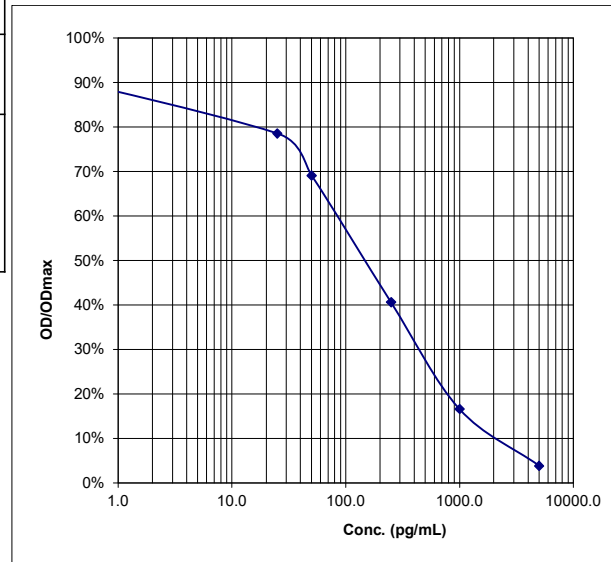

Kit Composition:

REF		LOT	
KEPR651	CONTROL 1	K330	2027-06
KEPR661	CONTROL 2	K331	2027-06
KEPR511	MTP	K326	2027-06
KEPR541	ENZCONJ	K327	2027-06
KEPR611	CAL A	K328	2027-06
KEPR621	CAL B-F	K329	2027-06
KIZZ01	CONC WASHBUF	K359	2029-03
KEZZ991	TMB SUBS	K132-5	2028-09

REF		LOT	
KEZZ921	TMB STOP	K356	2028-09

Valid edition of the instructions for use: 2024-12

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: T. Borchert

Validation date: 2025-10-15

Accepted

This document has been produced electronically and is valid without a signature.



IBL International GmbH
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11
E-MAIL: ibl@tecan.com
WEB: www.tecan.com/ibl