

Quality Control Certificate



Progesterone Saliva ELISA


REF RE52281	LOT EPR145	2028-02-29 YYYY-MM-DD
--------------------	-------------------	---------------------------------

Final Release Results:

	Concentration pg/mL	manual			e.g. automated EVOlyzer
		Measured value OD	Range* OD	OD/ODmax OD	Measured value OD
CAL A	0	2.100	> 1.000	100%	2.288
CAL B	25	1.709	-	81%	1.942
CAL C	50	1.562	-	74%	1.730
CAL D	250	1.070	-	51%	1.098
CAL E	1000	0.437	-	21%	0.460
CAL F	5000	0.105	-	5%	0.102

*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

Validation criteria				
	Concentration found pg/mL	Acceptable range		
		lower limit pg/mL	target pg/mL	upper limit pg/mL
CONTROL 1	61.9	43.2	61.7	80.3
CONTROL 2	685	444	634	824

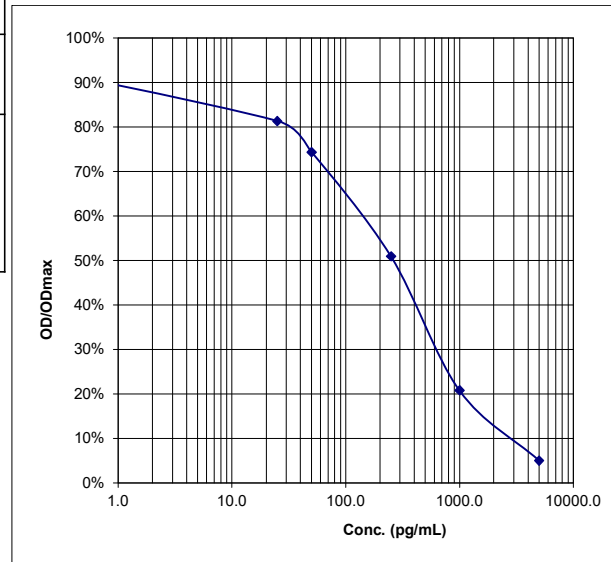

Kit Composition:

REF	LOT		REF	LOT	
KEPR651	CONTROL 1	K608	2028-02	KEZZ921	TMB STOP
KEPR661	CONTROL 2	K609	2028-02	K611	2029-03
KEPR511	MTP	K604	2028-02		
KEPR541	ENZCONJ	K605	2028-03		
KEPR611	CAL A	K606	2028-02		
KEPR621	CAL B-F	K607	2028-02		
KIZZ01	CONC WASHBUF	K612	2029-09		
KEZZ991	TMB SUBS	K610	2029-08		

Valid edition of the instructions for use: 2024-12

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: T. Borchert

Accepted

Validation date: 2026-06-25

This document has been produced electronically and is valid without a signature.