

# Quality Control Certificate



## Aldosterone ELISA


REF RE52301

LOT 89K065

2026-07-31  
YYYY-MM-DD

### Final Release Results:

|       | Concentration<br>pg/mL | Measured<br>value<br>OD | Range<br>OD | OD/ODmax |
|-------|------------------------|-------------------------|-------------|----------|
| CAL A | 0                      | 2.33                    | ≥ 1.20      | 100%     |
| CAL B | 20                     | 1.87                    | -           | 80%      |
| CAL C | 80                     | 1.08                    | -           | 46%      |
| CAL D | 200                    | 0.57                    | -           | 24%      |
| CAL E | 500                    | 0.27                    | -           | 12%      |
| CAL F | 1000                   | 0.15                    | -           | 6%       |

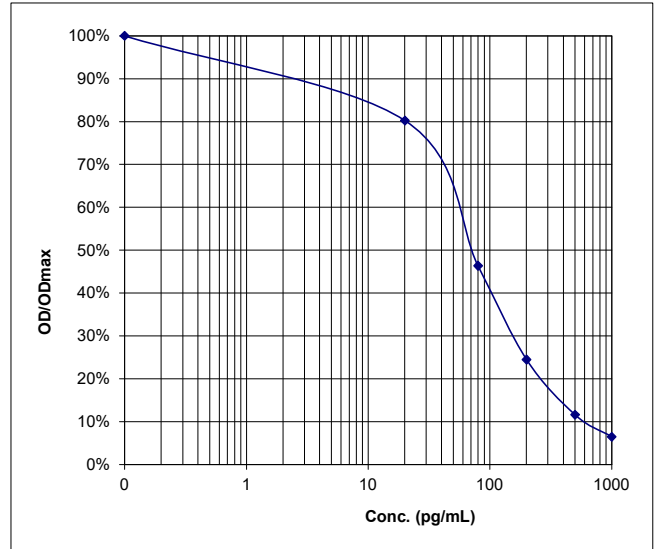

|              | Concentration<br>found<br>pg/mL | Target<br>Value<br>pg/mL | Acceptable range<br>lower limit<br>pg/mL | upper limit<br>pg/mL |
|--------------|---------------------------------|--------------------------|--|----------------------|
| Control Low  | 60.3                            | 52.7                     | 29.0                                     | 76.4                 |
| Control High | 436                             | 442                      | 243                                      | 641                  |

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: Dr. Spangenberg

Validation date: 2025-07-17

**Accepted**

This document has been produced electronically and is valid without a signature.



IBL International GmbH  
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11  
E-MAIL: [ibl@tecan.com](mailto:ibl@tecan.com)  
WEB: [www.tecan.com/ibl](http://www.tecan.com/ibl)