

Quality Control Certificate



DHEA Saliva ELISA


REF RE52651	LOT EDE132	2027-09-30 YYYY-MM-DD
--------------------	-------------------	---------------------------------

Final Release Results:

	Concentration pg/mL	manual		
		Measured value OD	Range* OD	OD/ODmax
CAL A	0	2.067	> 1.000	100%
CAL B	20	1.812	-	88%
CAL C	60	1.411	-	68%
CAL D	180	1.004	-	49%
CAL E	540	0.729	-	35%
CAL F	2160	0.310	-	15%

*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

Validation criteria (manual/automated)				
	Concentration found pg/mL	Acceptable range		
		lower limit pg/mL	target pg/mL	upper limit pg/mL
CONTROL 1	95	61	102	142
CONTROL 2	491	328	468	608

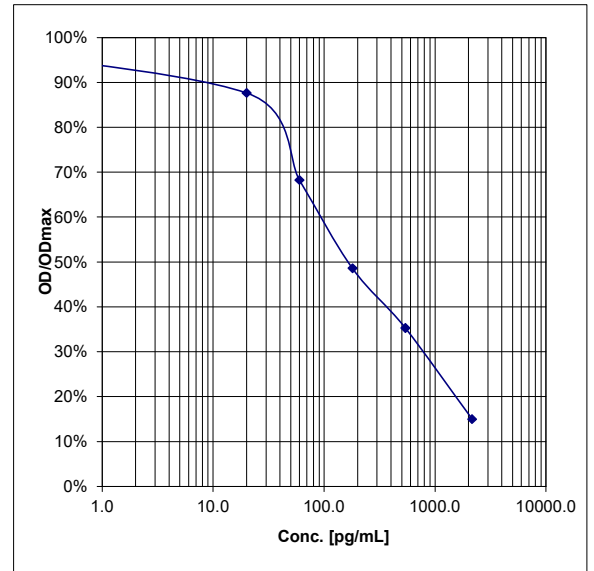

Kit Composition:

REF		LOT	
KEDE511	MTP	K376	2027-09
KEDE541	ENZCONJ	K389	2027-09
KEDE611	CAL A	K373	2027-09
KEDE621	CAL B-F	K373	2027-09
KEDE651	CONTROL 1	K374	2027-09
KEDE661	CONTROL 2	K375	2027-09
KEZZ991	TMB SUBS	K132-5	2028-09
KEZZ921	TMB STOP	K356	2028-09
KIZZ01	CONC WASHBUF	K387	2029-03

REF	LOT	

Valid edition of the instructions for use: 2024-08

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: Dr. Spangenberg

Accepted

Validation date: 2025-11-07

This document has been produced electronically and is valid without a signature.