

# Quality Control Certificate



## DHEA Saliva ELISA


<b>REF</b> RE52651	<b>LOT</b> EDE133	<b>2028-04-30</b> YYYY-MM-DD
--------------------	-------------------	---------------------------------

**Final Release Results:**

	Concentration pg/mL	Measured value OD	manual	
			Range*	OD/ODmax
CAL A	0	2.250	> 1.000	100%
CAL B	20	1.907	-	85%
CAL C	60	1.539	-	68%
CAL D	180	1.141	-	51%
CAL E	540	0.678	-	30%
CAL F	2160	0.356	-	16%

\*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

Validation criteria (manual/automated)				
	Concentration found pg/mL	Acceptable range		
		lower limit pg/mL	target pg/mL	upper limit pg/mL
CONTROL 1	102	56	93	130
CONTROL 2	459	301	430	559

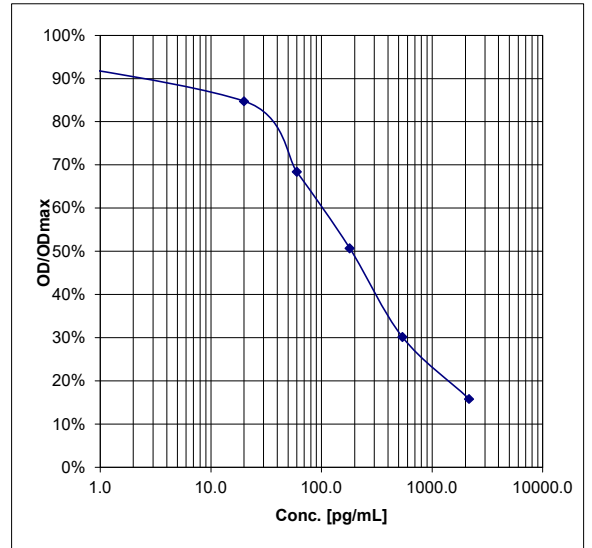

**Kit Composition:**

REF		LOT	
KEDE511	MTP	K761	2028-04
KEDE541	ENZCONJ	K762	2028-05
KEDE611	CAL A	K763	2028-05
KEDE621	CAL B-F	K763	2028-05
KEDE651	CONTROL 1	K764	2028-05
KEDE661	CONTROL 2	K765	2028-05
KEZZ991	TMB SUBS	K610	2029-08
KEZZ921	TMB STOP	K654	2029-03
KIZZ01	CONC WASHBUF	K766	2029-11

REF	LOT	
-----	-----	--

Valid edition of the instructions for use: 2024-08

**This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.**

Verified by: T. Borchert

**Accepted**

Validation date: 2026-06-24

This document has been produced electronically and is valid without a signature.