

# Quality Control Certificate




## Leptin ELISA

<b>REF</b> RE53151	<b>LOT</b> 45K046	<b>2027-11-12</b> YYYY-MM-DD
--------------------	-------------------	---------------------------------

### Final Release Results:

	Concentration ng/mL	Measured value OD	Range OD	OD/ODmax
CAL 0	0	0.05	-	2%
CAL 1	2	0.20	-	9%
CAL 2	5	0.41	-	19%
CAL 3	25	1.09	-	50%
CAL 4	50	1.64	-	75%
CAL 5	100	2.19	≥ 1.20	100%

	Concentration found ng/mL	Acceptable range		
		lower limit ng/mL	target ng/mL	upper limit ng/mL
CONTROL LOW	4.75	3.29	5.98	8.67
CONTROL HIGH	59.7	33.7	61.2	88.7

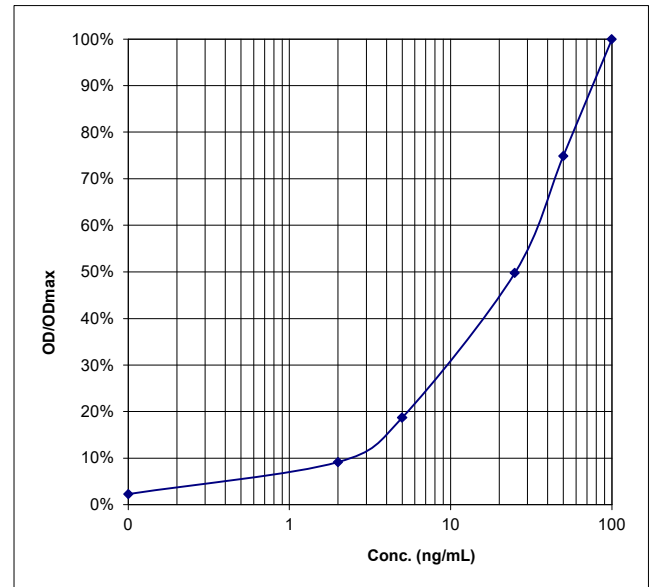

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: Dr. Spangenberg

Validation date: 2026-04-28

# Accepted

This document has been produced electronically and is valid without a signature.



**IBL International GmbH**  
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11  
E-MAIL: [ibl@tecan.com](mailto:ibl@tecan.com)  
WEB: [www.tecan.com/ibl](http://www.tecan.com/ibl)