

Quality Control Certificate



Serotonin high sensitive ELISA

REF RE59141


LOT SES120

2027-10-31
YYYY-MM-DD

Final Release Results:

	Calibrator concentration pg/sample	Measured value OD	Range OD	OD/ODmax
CAL A	0	1.568	-	100%
CAL B	0.67	1.378	-	88%
CAL C	2.0	1.051	-	67%
CAL D	6.7	0.663	-	42%
CAL E	20	0.374	-	24%
CAL F	100	0.169	-	11%

	Concentration found pg/sample	Acceptable range		
		lower limit pg/sample	target pg/sample	upper limit pg/sample
CONTROL 1	3.2	2.1	3.6	5.0
CONTROL 2	11.2	7.2	11.9	16.6

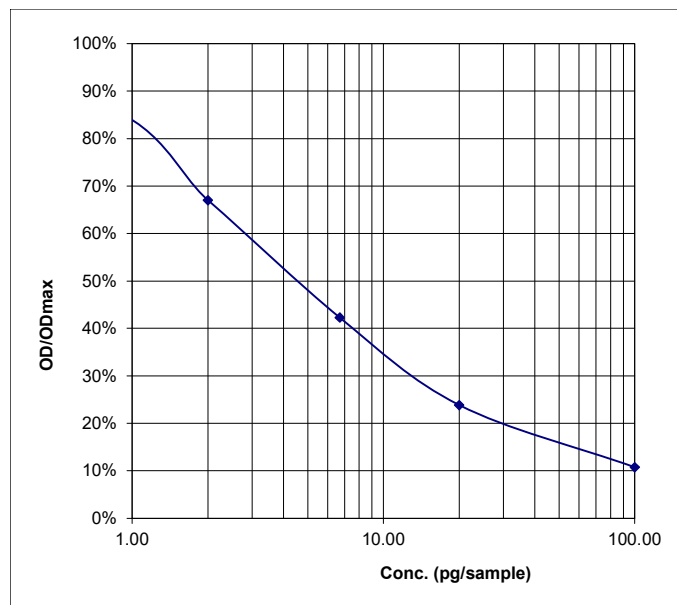

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: Dr. Spangenberg

Accepted

Validation date: 2026-08-31

This document has been produced electronically and is valid without a signature.



IBL International GmbH
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11
E-MAIL: ibl@tecan.com
WEB: www.tecan.com/ibl