

# Quality Control Certificate




## MetCombi Plasma ELISA (Metanephrine)

<b>REF</b> RE59202	<b>LOT</b> MNPE149	<b>2026-08-31</b> YYYY-MM-DD
--------------------	--------------------	---------------------------------

### Final Release Results:

	Concentration pg/mL	manual			automated e.g. DSX
		Measured value OD	Range OD	OD/ODmax	Measured value OD
CAL A	0	1.917	> 1.000	100%	2.443
CAL B	20	1.478	-	77%	1.914
CAL C	55	1.242	-	65%	1.517
CAL D	140	0.985	-	51%	1.141
CAL E	340	0.782	-	41%	0.989
CAL F	700	0.638	-	33%	0.825

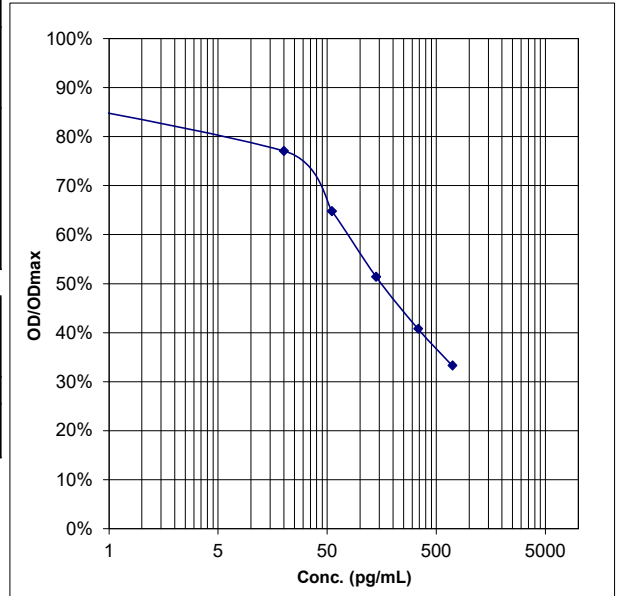

	Acceptable range			Concentration found	
	lower limit pg/mL	target pg/mL	upper limit pg/mL	pg/mL	
				manual	automated
CONTROL 1	49	81	113	89	89
CONTROL 2	157	261	365	262	268

\*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

### Kit Composition:

REF	LOT		REF	LOT	
KEWP501	MPMT47	MTP MN 2026-11	KEWP521	MPAS49	ANTISERUM MN 2026-08
KEWP611A	NPST45	LYO CAL A 2026-11	KEWP541	NPKJ47	ENZCONJ 2026-11
KEWP611	NPST45	LYO CAL B-F 2026-11	KEWP551	NPOS47	SOLVENT 2026-09
KEWP651	NPKO45	LYO CONTROL 1 2026-11	KEWP761	NPAP39	ACYLBUF 2029-03
KEWP661	NPKO45	LYO CONTROL 2 2026-11	KEWP791	NPPR43	PREC TUBES 2026-11
KEWP771	NPP140	PREC REAG 1 2028-10	KEWP561	NPWP31	WASHBUF CONC 2028-04
KEWP781	NPP243	PREC REAG 2 2027-07	KEWP571	NPSU48	TMB SUBS 2026-11
KEWP751	NPAR47	LYO ACYLREAG 2026-11	KEWP581	NPSO42	TMB STOP 2028-10

Valid edition of the instructions for use: Ver.8 / 07-2024

**This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.**

Verified by: Dr. Spangenberg

**Accepted**

Validation date: 2025-02-05

This document has been produced electronically and is valid without a signature.