

Quality Control Certificate




MetCombi Plasma ELISA (Normetanephrine)

REF RE59202	LOT MNPE149	2026-08-31 YYYY-MM-DD
--------------------	--------------------	---------------------------------

Final Release Results:

	Concentration pg/mL	manual			e.g. automated/ DSX
		Measured value OD	Range OD	OD/ODmax	Measured value OD
CAL A	0	1.504	> 1.000	100%	2.279
CAL B	30	1.214	-	81%	1.921
CAL C	65	0.935	-	62%	1.496
CAL D	120	0.725	-	48%	1.124
CAL E	240	0.532	-	35%	0.823
CAL F	500	0.413	-	27%	0.654

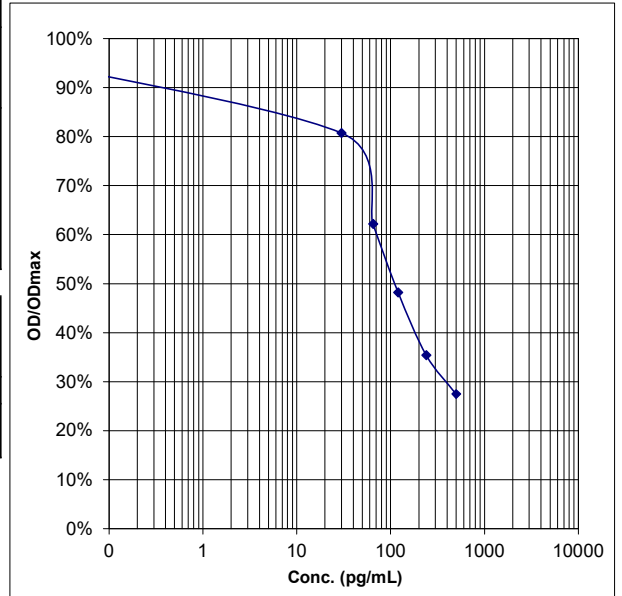

	Acceptable range			Concentration found	
	lower limit pg/mL	target pg/mL	upper limit pg/mL	manual	automated
CONTROL 1	58	97	136	94	102
CONTROL 2	108	180	252	186	172

*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

Kit Composition:

REF	LOT		REF	LOT	
KEWP511	MTP NMN	NPMT47 2026-11	KEWP531	ANTISERUM NMN	NPAS49 2026-08
KEWP611A	LYO CAL A	NPST45 2026-11	KEWP541	ENZCONJ	NPKJ47 2026-11
KEWP611	LYO CAL B-F	NPST45 2026-11	KEWP551	SOLVENT	NPOS47 2026-09
KEWP651	LYO CONTROL 1	NPKO45 2026-11	KEWP761	ACYLBUF	NPAP39 2029-03
KEWP661	LYO CONTROL 2	NPKO45 2026-11	KEWP791	PREC TUBES	NPPR43 2026-11
KEWP771	PREC REAG 1	NPP140 2028-10	KEWP561	WASHBUF CONC	NPWP31 2028-04
KEWP781	PREC REAG 2	NPP243 2027-07	KEWP571	TMB SUBS	NPSU48 2026-11
KEWP751	LYO ACYLREAG	NPAR47 2026-11	KEWP581	TMB STOP	NPSO42 2028-10

Valid edition of the instructions for use: Ver.8 / 07-2024

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: Dr. Spangenberg

Accepted

Validation date: 2025-02-05

This document has been produced electronically and is valid without a signature.