

# Quality Control Certificate




## MetCombi Plasma ELISA (Normetanephrine)

<b>REF</b> RE59202	<b>LOT</b> MNPE153	<b>2027-12-31</b> YYYY-MM-DD
--------------------	--------------------	---------------------------------

### Final Release Results:

	Concentration pg/mL	manual			e.g. automated/ DSX
		Measured value OD	Range OD	OD/ODmax	Measured value OD
CAL A	0	1.871	> 1.000	100%	2.124
CAL B	30	1.541	-	82%	1.722
CAL C	65	1.302	-	70%	1.443
CAL D	130	0.982	-	52%	1.019
CAL E	270	0.744	-	40%	0.804
CAL F	750	0.559	-	30%	0.605

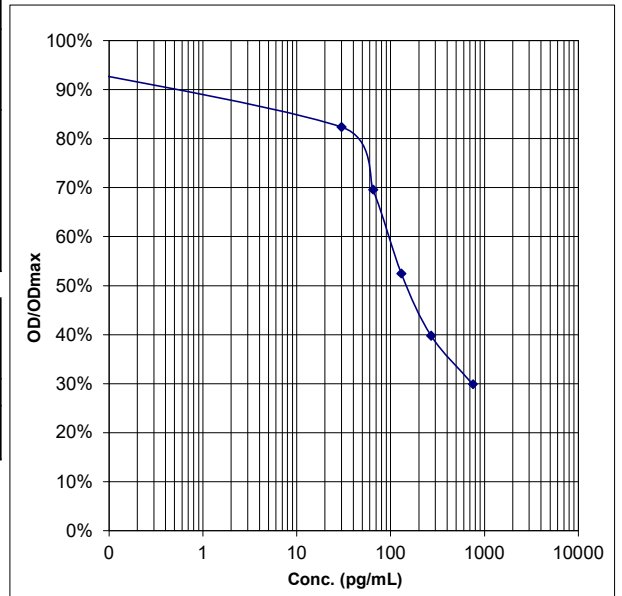

	Acceptable range			Concentration found	
	lower limit pg/mL	target pg/mL	upper limit pg/mL	manual	automated
CONTROL 1	61	102	143	105	122
CONTROL 2	122	203	284	228	228

\*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

### Kit Composition:

REF	LOT	Icon	REF	LOT	Icon
KEWP511	MTP NMN		KEWP531	ANTISERUM NMN	
KEWP611A	LYO CAL A		KEWP541	ENZCONJ	
KEWP611	LYO CAL B-F		KEWP551	SOLVENT	
KEWP651	LYO CONTROL 1		KEWP761	ACYLBUF	
KEWP661	LYO CONTROL 2		KEWP791	PREC TUBES	
KEWP771	PREC REAG 1		KEWP561	WASHBUF CONC	
KEWP781	PREC REAG 2		KEWP571	TMB SUBS	
KEWP751	LYO ACYLREAG		KEWP581	TMB STOP	

Valid edition of the instructions for use: Version 10, Dez-2025

**This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.**

Verified by: **Dr. Spangenberg**

**Accepted**

Validation date: **2026-06-09**

This document has been produced electronically and is valid without a signature.



**IBL International GmbH**  
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11  
E-MAIL: [ibl@tecan.com](mailto:ibl@tecan.com)  
WEB: [www.tecan.com/ibl](http://www.tecan.com/ibl)