

# Quality Control Certificate



## TriCat TM ELISA (Dopamine)


<b>REF</b> RE59395	<b>LOT</b> ETC162	<b>2026-06-30</b> YYYY-MM-DD
--------------------	-------------------	---------------------------------

### Final Release Results:

	Concentration ng/mL	manual		e.g. automated/ EVOlyzer
		Measured value OD	OD/ODmax	Measured value OD
CAL A	0	0.096	5%	0.134
CAL B	60	0.168	9%	0.265
CAL C	180	0.284	14%	0.510
CAL D	585	0.678	34%	0.909
CAL E	2300	1.444	73%	1.823
CAL F	11470	1.973	100%	2.377

	Concentration found ng/mL	Acceptable range		
		lower limit ng/mL	target ng/mL	upper limit ng/mL
CONTROL 1	157	98	163	228
CONTROL 2	649	360	600	840

\*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

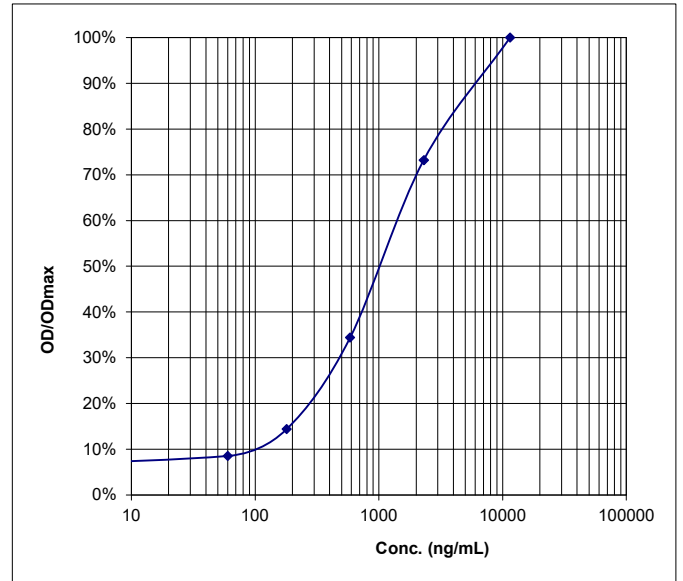

### Kit Composition:

REF	LOT		REF	LOT			
KEZZ521	CONTROL 1	K212	2027-06	KEZZ575	LYO COMT	K204	2026-06
KEZZ531	CONTROL 2	K213	2027-06	KEZZ581	COENZ	K203	2026-06
KEZZ801	MTP	K209	2028-06	KEZZ591	ENZBUF	K201	2028-06
KEZZ431	ANTISERUM DO	K207	2026-07	KEZZ422	COMT ADD	K202	2026-07
KEZZ821	CONC ENZCONJ	K214	2027-07	KEZZ609	RELEASEBUF	K200	2026-07
KEZZ511	CAL A-F	K211	2027-06	KLZZ879	CONC WASHBUF	K215	2027-06
KEZZ541	ACYLREAG	K208	2026-07	KEZZ971	PNPP SUBS	L747-4	2026-08
KEZZ555	EXTRPLATE	K210	2027-06	KEZZ951	PNPP STOP	K216	2028-06
KEZZ565	EXTRBUF	K199	2026-07				

Valid edition of the instructions for use: 2015-07

**This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.**

Verified by: T.Schmidt

Accepted

Validation date: 2025-09-01

This document has been produced electronically and is valid without a signature.