

Quality Control Certificate



TriCat TM ELISA (Noradrenalin)


REF RE59395	LOT ETC163	2027-02-28 YYYY-MM-DD
--------------------	-------------------	---------------------------------

Final Release Results:

	Concentration ng/mL	manual		e.g. automated/ EVOlyzer
		Measured value OD	OD/ODmax	Measured value OD
CAL A	0	0.071	3%	0.132
CAL B	5.0	0.218	9%	0.286
CAL C	15	0.473	20%	0.562
CAL D	50	1.149	48%	1.320
CAL E	150	1.827	76%	1.995
CAL F	500	2.399	100%	2.527

	Concentration found ng/mL	Acceptable range		
		lower limit ng/mL	target ng/mL	upper limit ng/mL
CONTROL 1	20.1	15.2	22.3	29.5
CONTROL 2	109	73	107	141

*During automated procedure the optical densities of calibrators and controls may rise due to temperature and specific device conditions. In case of none conformance with the OD ranges stated on the QC Certificate please contact IBL-International or use the validation criteria only!

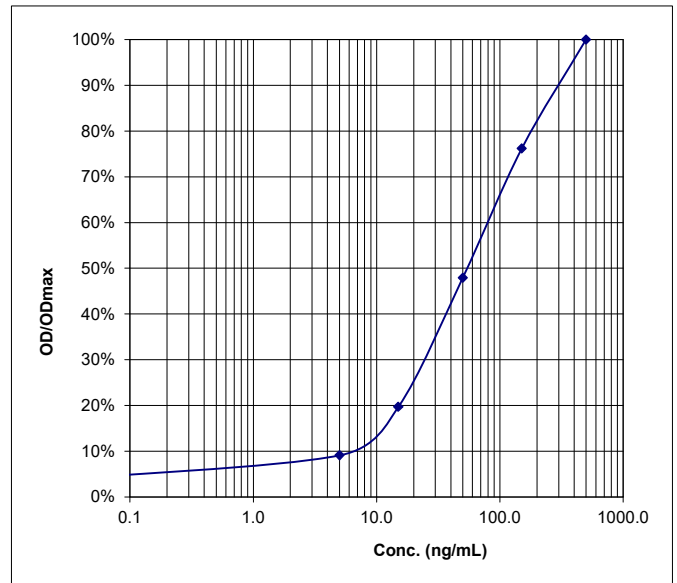

Kit Composition:

REF	LOT		REF	LOT	
KEZZ521	K627	CONTROL 1	KEZZ575	K622	LYO COMT
KEZZ531	K628	CONTROL 2	KEZZ581	K621	COENZ
KEZZ801	K614	MTP	KEZZ591	K619	ENZBUF
KEZZ411	K617	ANTISERUM NAD	KEZZ422	K620	COMT ADD
KEZZ821	K629	CONC ENZCONJ	KEZZ601/9	K624	RELEASEBUF
KEZZ511	K626	CAL A-F	KLZZ879	K586	CONC WASHBUF
KEZZ541	K623	ACYLREAG	KEZZ971	K492-3	PNPP SUBS
KEZZ555	K615	EXTRPLATE	KEZZ951	K630	PNPP STOP
KEZZ565	K625	EXTRBUF			

Valid edition of the instructions for use: 2015-07

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: **S. Geweke**

Validation date: **2026-04-23**

Accepted

This document has been produced electronically and is valid without a signature.