

Quality Control Certificate




IRT Neonatal Luminescence Immunoassay

REF	RE68019	LOT	LIT206	 2028-06-30 YYYY-MM-DD
-----	---------	-----	--------	---

Final Release Results:

	Concentration ng/mL	Measured value RLU	Range RLU	RLU/RLUmax
CAL A	0	52790	-	4%
CAL B	24	115660	-	8%
CAL C	48	224430	-	16%
CAL D	105	426380	-	31%
CAL E	190	955390	-	69%
CAL F	360	1376680	-	100%

	Concentration found ng/mL	Acceptable range		
		lower limit ng/mL	target ng/mL	upper limit ng/mL
CONTROL 1	93	57	81	105
CONTROL 2	147	95	136	177

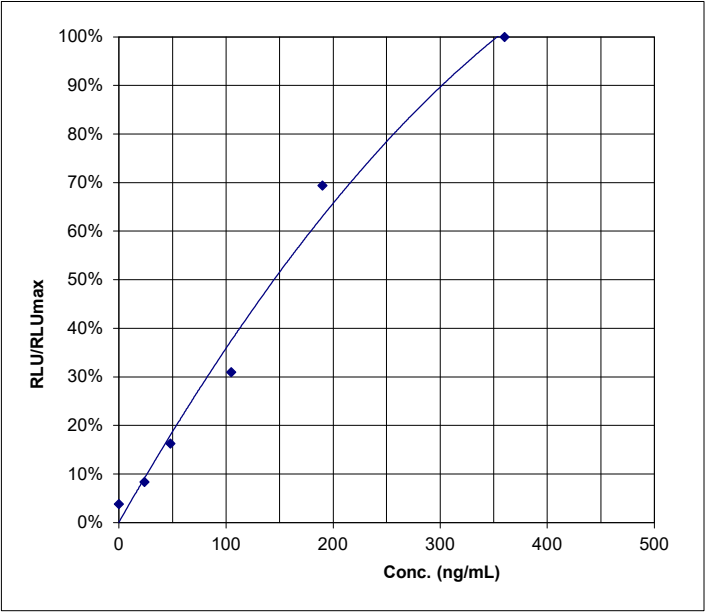

Kit Composition:

REF		LOT	
KLIT655	CONTROL 1	303	2028-06
KLIT665	CONTROL 2	304	2028-06
KLIT511	MTP	K857	2028-06
KLIT545	CONC ENZCONJ	K890	2028-07
KLIT615	CAL A-F	302	2028-06

REF		LOT	
KLIT755	CONC ASSAYBUF	K860	2028-06
KLZZ635	LUMINREAG	K878	2028-06
KLZZ879	CONC WASHBUF	K852	2028-06

Valid edition of the instructions for use: 2024-10

This product has been tested successfully by the Quality Control Department and was released for sale according to the existing specifications.

Verified by: Dr. Spangenberg

Validation date: 2026-07-22

Accepted

This document has been produced electronically and is valid without a signature.